

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019087.D
 Acq On : 23 Oct 2020 11:07
 Operator : SY/MD
 Sample : VV1023MBL01
 Misc : 5.00G/5uL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK95

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB	176707	181824	14.95%	1.977%
2	1.576	144	151	161	rVB	156458	172537	14.18%	1.876%
3	2.119	310	320	351	rVB	297906	461327	37.92%	5.016%
4	2.528	438	447	452	rBV4	1207	1923	0.16%	0.021%
5	2.753	514	517	520	rVB	290	153	0.01%	0.002%
6	2.868	549	553	556	rBV	283	223	0.02%	0.002%
7	2.946	575	577	578	rBV	280	108	0.01%	0.001%
8	3.000	591	594	596	rBV	244	167	0.01%	0.002%
9	3.077	614	618	621	rVB2	248	110	0.01%	0.001%
10	3.097	621	624	625	rBV	319	210	0.02%	0.002%
11	3.145	635	639	642	rBV2	243	221	0.02%	0.002%
12	3.174	644	648	651	rVB	455	306	0.03%	0.003%
13	3.193	651	654	655	rBV	169	100	0.01%	0.001%
14	3.245	667	670	676	rBV2	312	294	0.02%	0.003%
15	3.492	743	747	749	rBV	267	227	0.02%	0.002%
16	3.579	771	774	782	rBV2	264	253	0.02%	0.003%
17	3.637	790	792	796	rVB2	244	145	0.01%	0.002%
18	3.714	815	816	817	rBV2	153	46	0.00%	0.001%
19	3.730	817	821	823	rVV2	273	212	0.02%	0.002%
20	3.772	832	834	837	rBV	254	110	0.01%	0.001%
21	3.788	837	839	842	rBV	163	86	0.01%	0.001%
22	3.856	858	860	861	rVB	173	42	0.00%	0.000%
23	3.913	867	878	918	rBV	83324	261483	21.50%	2.843%
24	4.373	1005	1021	1048	rBV	198714	485076	39.88%	5.275%
25	4.663	1109	1111	1114	rBV2	537	395	0.03%	0.004%
26	4.724	1128	1130	1132	rVB2	293	89	0.01%	0.001%
27	4.939	1195	1197	1199	rBV	163	91	0.01%	0.001%
28	4.997	1211	1215	1218	rBV	522	508	0.04%	0.006%
29	5.071	1221	1238	1265	rBV2	476159	1216437	100.00%	13.227%
30	5.386	1331	1336	1337	rBV	315	196	0.02%	0.002%
31	5.428	1346	1349	1353	rBV3	473	301	0.02%	0.003%
32	5.495	1368	1370	1373	rBV	220	94	0.01%	0.001%
33	5.640	1402	1415	1441	rBV	352313	708017	58.20%	7.699%
34	5.907	1495	1498	1499	rBV2	181	111	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019087.D
 Acq On : 23 Oct 2020 11:07
 Operator : SY/MD
 Sample : VV1023MBL01
 Misc : 5.00G/5uL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK95

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

35	5.997	1524	1526	1527	rBV2	231	95	0.01%	0.001%
36	6.093	1540	1556	1577	rBV	275239	558572	45.92%	6.074%
37	6.351	1632	1636	1641	rBV2	392	349	0.03%	0.004%
38	6.383	1641	1646	1648	rBV2	225	189	0.02%	0.002%
39	6.428	1656	1660	1661	rBV	278	164	0.01%	0.002%
40	6.473	1672	1674	1677	rBV	354	194	0.02%	0.002%
41	6.524	1687	1690	1695	rBV3	454	436	0.04%	0.005%
42	6.592	1708	1711	1714	rBV	367	244	0.02%	0.003%
43	6.627	1718	1722	1726	rBV2	253	223	0.02%	0.002%
44	6.659	1726	1732	1738	rBV2	356	506	0.04%	0.006%
45	6.704	1743	1746	1747	rBV2	342	155	0.01%	0.002%
46	6.749	1758	1760	1761	rBV2	119	40	0.00%	0.000%
47	6.862	1792	1795	1798	rBV2	246	188	0.02%	0.002%
48	6.929	1814	1816	1817	rBV	168	51	0.00%	0.001%
49	6.962	1823	1826	1828	rBV2	234	132	0.01%	0.001%
50	7.007	1828	1840	1866	rBV	151607	277955	22.85%	3.022%
51	7.296	1928	1930	1931	rBV	377	142	0.01%	0.002%
52	7.338	1931	1943	1970	rVV	537553	927636	76.26%	10.087%
53	7.640	2027	2037	2068	rBV	111430	198221	16.30%	2.155%
54	7.852	2101	2103	2104	rBV	270	99	0.01%	0.001%
55	7.878	2109	2111	2114	rBV	260	167	0.01%	0.002%
56	7.952	2129	2134	2136	rBV2	430	400	0.03%	0.004%
57	8.010	2148	2152	2155	rBV2	413	333	0.03%	0.004%
58	8.106	2172	2182	2215	rBV	325960	566395	46.56%	6.159%
59	8.434	2279	2284	2298	rBV6	1564	2814	0.23%	0.031%
60	8.540	2315	2317	2319	rBV2	237	124	0.01%	0.001%
61	8.701	2364	2367	2369	rBV	345	172	0.01%	0.002%
62	8.772	2387	2389	2390	rBV	336	124	0.01%	0.001%
63	8.871	2409	2420	2445	rBV	546706	896085	73.66%	9.744%
64	9.035	2469	2471	2476	rBV2	402	386	0.03%	0.004%
65	9.437	2594	2596	2599	rBV2	303	164	0.01%	0.002%
66	9.473	2605	2607	2610	rVB	230	108	0.01%	0.001%
67	9.534	2621	2626	2629	rBV2	360	328	0.03%	0.004%
68	9.559	2631	2634	2636	rBV	271	164	0.01%	0.002%
69	9.611	2648	2650	2653	rVB2	346	132	0.01%	0.001%
70	9.691	2673	2675	2676	rBV	297	134	0.01%	0.001%
71	9.823	2710	2716	2717	rBV	247	266	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019087.D
 Acq On : 23 Oct 2020 11:07
 Operator : SY/MD
 Sample : VV1023MBL01
 Misc : 5.00G/5uL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK95

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

72	9.955	2755	2757	2760	rBV2	300	201	0.02%	0.002%
73	9.984	2763	2766	2768	rBV	228	152	0.01%	0.002%
74	10.042	2781	2784	2787	rBV	246	168	0.01%	0.002%
75	10.235	2832	2844	2864	rBV	353740	555042	45.63%	6.035%
76	10.444	2907	2909	2913	rVB2	601	357	0.03%	0.004%
77	10.473	2913	2918	2922	rBV2	279	309	0.03%	0.003%
78	10.489	2922	2923	2925	rVB2	238	68	0.01%	0.001%
79	10.505	2925	2928	2929	rBV	185	98	0.01%	0.001%
80	10.540	2936	2939	2940	rBV	321	147	0.01%	0.002%
81	10.704	2986	2990	2994	rBV2	409	367	0.03%	0.004%
82	10.759	3003	3007	3010	rBV	480	438	0.04%	0.005%
83	10.878	3041	3044	3047	rBV2	285	185	0.02%	0.002%
84	10.920	3055	3057	3058	rBV2	237	96	0.01%	0.001%
85	10.952	3062	3067	3069	rBV4	333	297	0.02%	0.003%
86	11.103	3111	3114	3116	rBV	315	244	0.02%	0.003%
87	11.270	3155	3166	3195	rBV	543357	831973	68.39%	9.047%
88	11.460	3223	3225	3229	rVB	395	209	0.02%	0.002%
89	11.524	3242	3245	3248	rBV2	358	260	0.02%	0.003%
90	11.595	3266	3267	3270	rVB	260	93	0.01%	0.001%
91	11.646	3270	3283	3303	rBV	563178	877649	72.15%	9.543%
92	12.148	3435	3439	3443	rVB3	420	386	0.03%	0.004%
93	12.257	3470	3473	3474	rBV	291	173	0.01%	0.002%
94	12.656	3594	3597	3600	rBV3	364	251	0.02%	0.003%


Sum of corrected areas: 9196472

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102320\
Data File : VV019087.D
Acq On : 23 Oct 2020 11:07
Operator : SY/MD
Sample : VV1023MBL01
Misc : 5.00G/5uL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK95

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

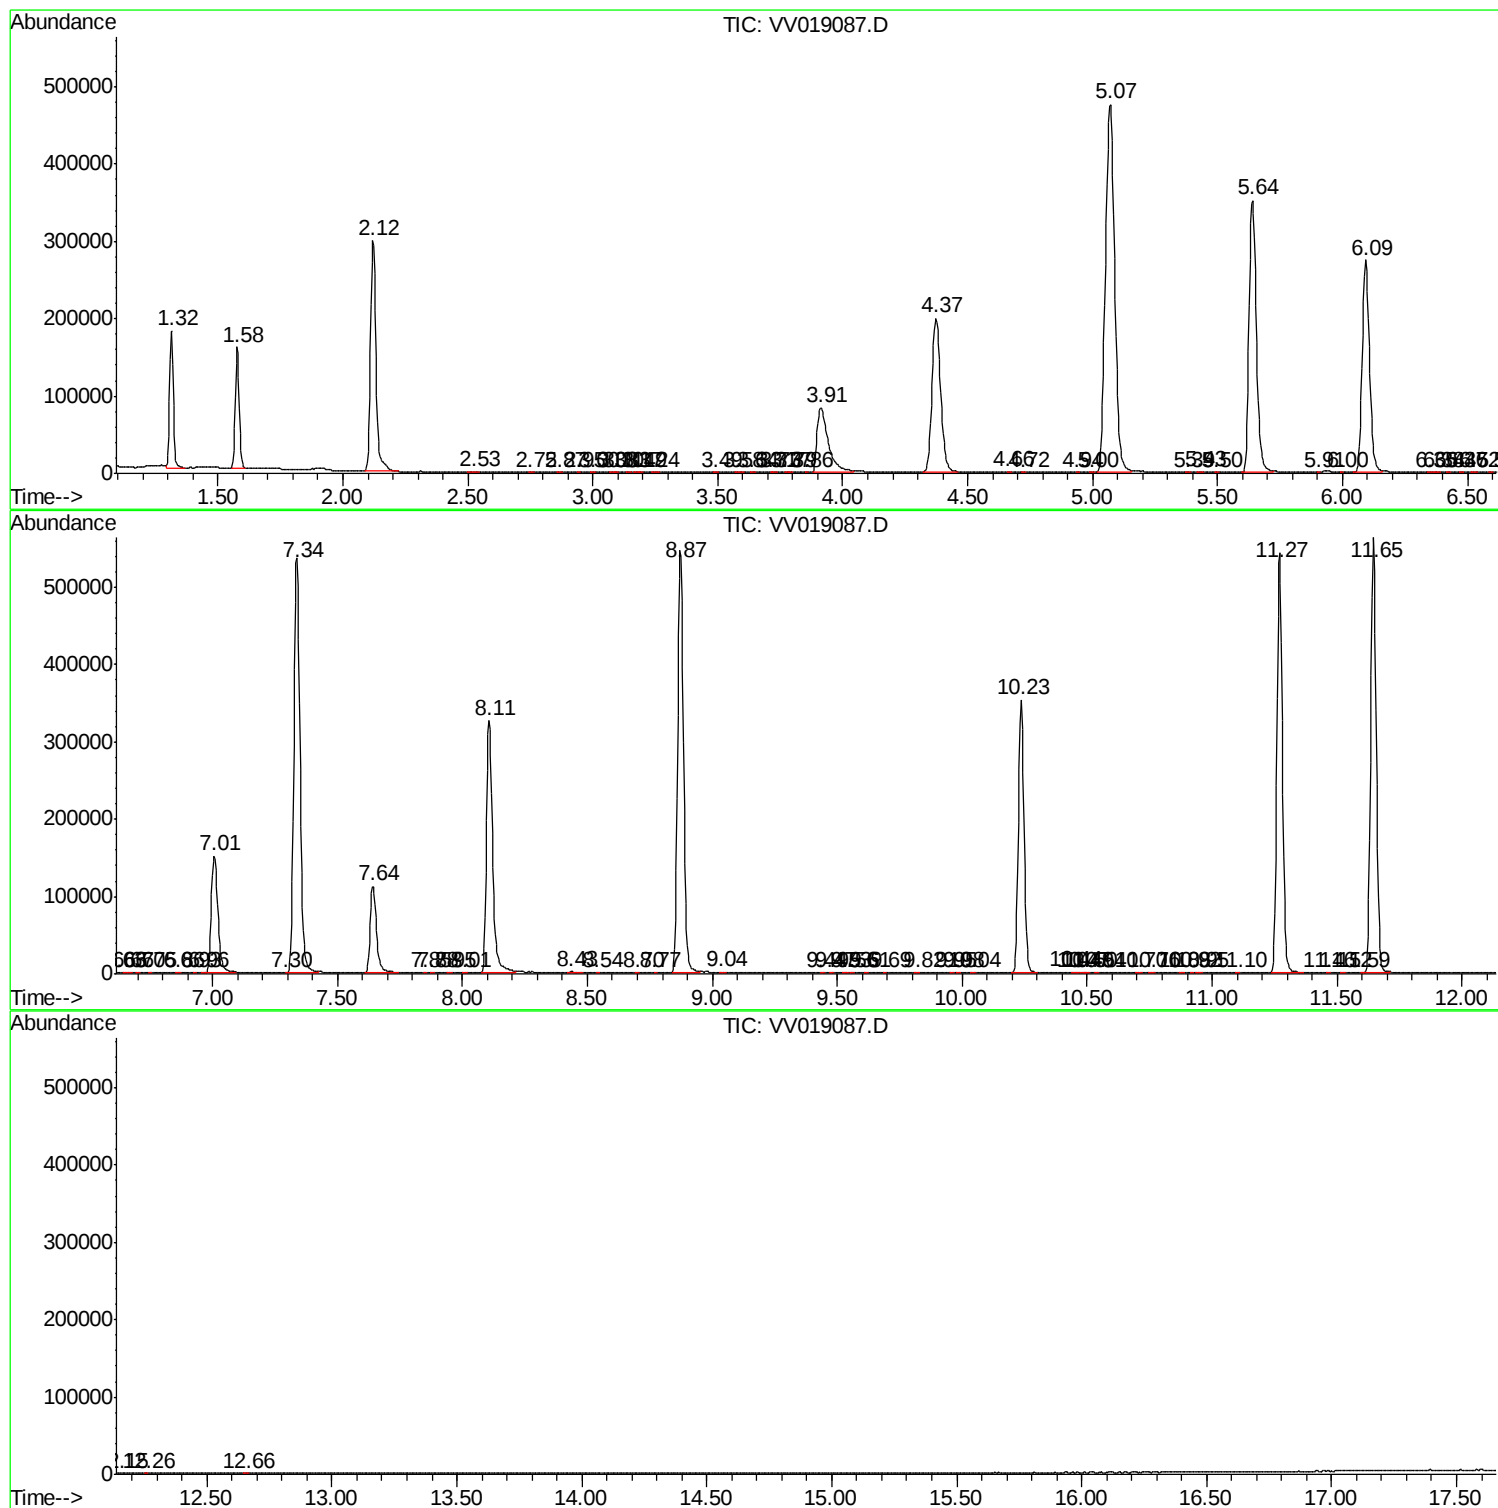

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102320\
Data File : VV019087.D
Acq On : 23 Oct 2020 11:07
Operator : SY/MD
Sample : VV1023MBL01
Misc : 5.00G/5uL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK95

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV102320\
Data File : VV019087.D
Acq On : 23 Oct 2020 11:07
Operator : SY/MD
Sample : VV1023MBL01
Misc : 5.00G/5uL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK95

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc