

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019090.D
 Acq On : 23 Oct 2020 14:26
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	88	rVB	164546	168573	14.59%	1.906%
2	1.579	145	152	168	rVB	144432	160261	13.87%	1.812%
3	2.122	311	321	351	rVB	282749	432182	37.40%	4.886%
4	2.592	464	467	469	rBV	344	212	0.02%	0.002%
5	2.630	477	479	482	rBV2	239	171	0.01%	0.002%
6	2.669	487	491	493	rBV	316	245	0.02%	0.003%
7	2.775	522	524	528	rBV2	213	138	0.01%	0.002%
8	2.878	552	556	559	rBV	215	137	0.01%	0.002%
9	2.923	566	570	572	rBV2	326	299	0.03%	0.003%
10	2.965	580	583	586	rVB2	383	280	0.02%	0.003%
11	3.145	637	639	640	rBV	252	90	0.01%	0.001%
12	3.267	673	677	681	rBV2	225	201	0.02%	0.002%
13	3.309	687	690	693	rBV	167	103	0.01%	0.001%
14	3.392	714	716	722	rBV2	278	221	0.02%	0.002%
15	3.437	727	730	732	rBV2	113	67	0.01%	0.001%
16	3.470	737	740	741	rBV	170	96	0.01%	0.001%
17	3.518	752	755	758	rVB	128	72	0.01%	0.001%
18	3.534	758	760	762	rBV2	181	121	0.01%	0.001%
19	3.659	796	799	802	rBV	267	224	0.02%	0.003%
20	3.756	826	829	831	rBV	232	129	0.01%	0.001%
21	3.785	834	838	840	rVB	295	185	0.02%	0.002%
22	3.801	840	843	845	rBV	399	235	0.02%	0.003%
23	3.817	846	848	851	rVB	333	186	0.02%	0.002%
24	3.859	858	861	863	rBV2	130	88	0.01%	0.001%
25	3.872	863	865	868	rVB	209	103	0.01%	0.001%
26	3.920	868	880	920	rBV	70404	248035	21.46%	2.804%
27	4.280	990	992	993	rBV	301	112	0.01%	0.001%
28	4.370	1004	1020	1048	rBV	185221	461209	39.91%	5.214%
29	4.579	1083	1085	1088	rVB	270	138	0.01%	0.002%
30	4.653	1105	1108	1112	rBV2	459	344	0.03%	0.004%
31	4.730	1129	1132	1136	rBV2	442	322	0.03%	0.004%
32	4.785	1146	1149	1150	rBV2	373	211	0.02%	0.002%
33	4.826	1157	1162	1165	rBV2	261	247	0.02%	0.003%
34	4.843	1165	1167	1172	rVV2	243	161	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019090.D
 Acq On : 23 Oct 2020 14:26
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

35	4.913	1186	1189	1192	rVB	370	225	0.02%	0.003%
36	4.990	1212	1213	1217	rVB	267	142	0.01%	0.002%
37	5.068	1219	1237	1265	rBV2	451320	1155578	100.00%	13.063%
38	5.508	1371	1374	1375	rBV	158	95	0.01%	0.001%
39	5.524	1378	1379	1380	rVV	271	60	0.01%	0.001%
40	5.534	1380	1382	1384	rVB	239	84	0.01%	0.001%
41	5.550	1384	1387	1389	rBV	207	129	0.01%	0.001%
42	5.637	1402	1414	1440	rBV	345193	694094	60.06%	7.846%
43	5.900	1492	1496	1497	rBV2	259	190	0.02%	0.002%
44	5.933	1498	1506	1521	rVB4	2206	4699	0.41%	0.053%
45	5.990	1521	1524	1526	rBV	122	81	0.01%	0.001%
46	6.023	1529	1534	1536	rBV2	262	229	0.02%	0.003%
47	6.090	1541	1555	1577	rBV	260257	526833	45.59%	5.956%
48	6.289	1615	1617	1619	rBV	241	84	0.01%	0.001%
49	6.479	1672	1676	1677	rBV	294	158	0.01%	0.002%
50	6.521	1685	1689	1693	rBV	293	295	0.03%	0.003%
51	6.675	1735	1737	1741	rBV	247	133	0.01%	0.002%
52	6.704	1743	1746	1747	rBV	259	115	0.01%	0.001%
53	6.717	1747	1750	1753	rVB	356	171	0.01%	0.002%
54	6.871	1797	1798	1799	rVB	215	41	0.00%	0.000%
55	6.884	1799	1802	1804	rBV	186	127	0.01%	0.001%
56	6.920	1810	1813	1815	rBV	126	79	0.01%	0.001%
57	6.936	1815	1818	1821	rVV	241	180	0.02%	0.002%
58	7.006	1828	1840	1863	rBV	143942	264685	22.90%	2.992%
59	7.215	1900	1905	1906	rBV2	415	366	0.03%	0.004%
60	7.286	1925	1927	1930	rBV2	318	148	0.01%	0.002%
61	7.334	1930	1942	1967	rBV	522530	897810	77.69%	10.149%
62	7.588	2013	2021	2027	rBV6	3665	5536	0.48%	0.063%
63	7.640	2027	2037	2062	rVV	108307	186850	16.17%	2.112%
64	7.875	2108	2110	2113	rVB	395	146	0.01%	0.002%
65	8.000	2147	2149	2152	rVB2	376	196	0.02%	0.002%
66	8.048	2160	2164	2168	rBV2	182	216	0.02%	0.002%
67	8.106	2168	2182	2209	rBV	311848	528890	45.77%	5.979%
68	8.437	2279	2285	2295	rBV6	1129	1938	0.17%	0.022%
69	8.746	2379	2381	2382	rBV6	166	54	0.00%	0.001%
70	8.801	2396	2398	2401	rBV	235	129	0.01%	0.001%
71	8.871	2408	2420	2440	rBV	542505	866868	75.02%	9.800%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019090.D
 Acq On : 23 Oct 2020 14:26
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

72	9.119	2495	2497	2502	rBV2	248	144	0.01%	0.002%
73	9.141	2502	2504	2506	rBV	230	80	0.01%	0.001%
74	9.231	2529	2532	2533	rBV2	115	65	0.01%	0.001%
75	9.341	2563	2566	2567	rBV	145	62	0.01%	0.001%
76	9.354	2567	2570	2572	rBV	194	141	0.01%	0.002%
77	9.566	2635	2636	2637	rBV	263	72	0.01%	0.001%
78	9.945	2749	2754	2756	rBV2	441	401	0.03%	0.005%
79	10.235	2832	2844	2863	rBV	331938	525606	45.48%	5.942%
80	10.334	2873	2875	2877	rBV	341	162	0.01%	0.002%
81	10.492	2921	2924	2926	rBV	327	229	0.02%	0.003%
82	10.601	2951	2958	2966	rVB3	3941	5744	0.50%	0.065%
83	10.736	2997	3000	3002	rBV	317	217	0.02%	0.002%
84	10.881	3039	3045	3050	rVB3	403	457	0.04%	0.005%
85	10.916	3053	3056	3058	rBV2	253	142	0.01%	0.002%
86	11.270	3154	3166	3187	rBV	549025	843504	72.99%	9.535%
87	11.424	3212	3214	3217	rVB	337	168	0.01%	0.002%
88	11.646	3270	3283	3302	rBV	538910	853851	73.89%	9.652%
89	11.900	3359	3362	3363	rBV	322	165	0.01%	0.002%
90	12.341	3493	3499	3502	rBV	480	477	0.04%	0.005%
91	13.283	3789	3792	3793	rBV	752	428	0.04%	0.005%
92	13.816	3956	3958	3964	rBV2	585	615	0.05%	0.007%
93	13.955	3998	4001	4003	rVB2	462	241	0.02%	0.003%


Sum of corrected areas: 8846023

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102320\
Data File : VV019090.D
Acq On : 23 Oct 2020 14:26
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

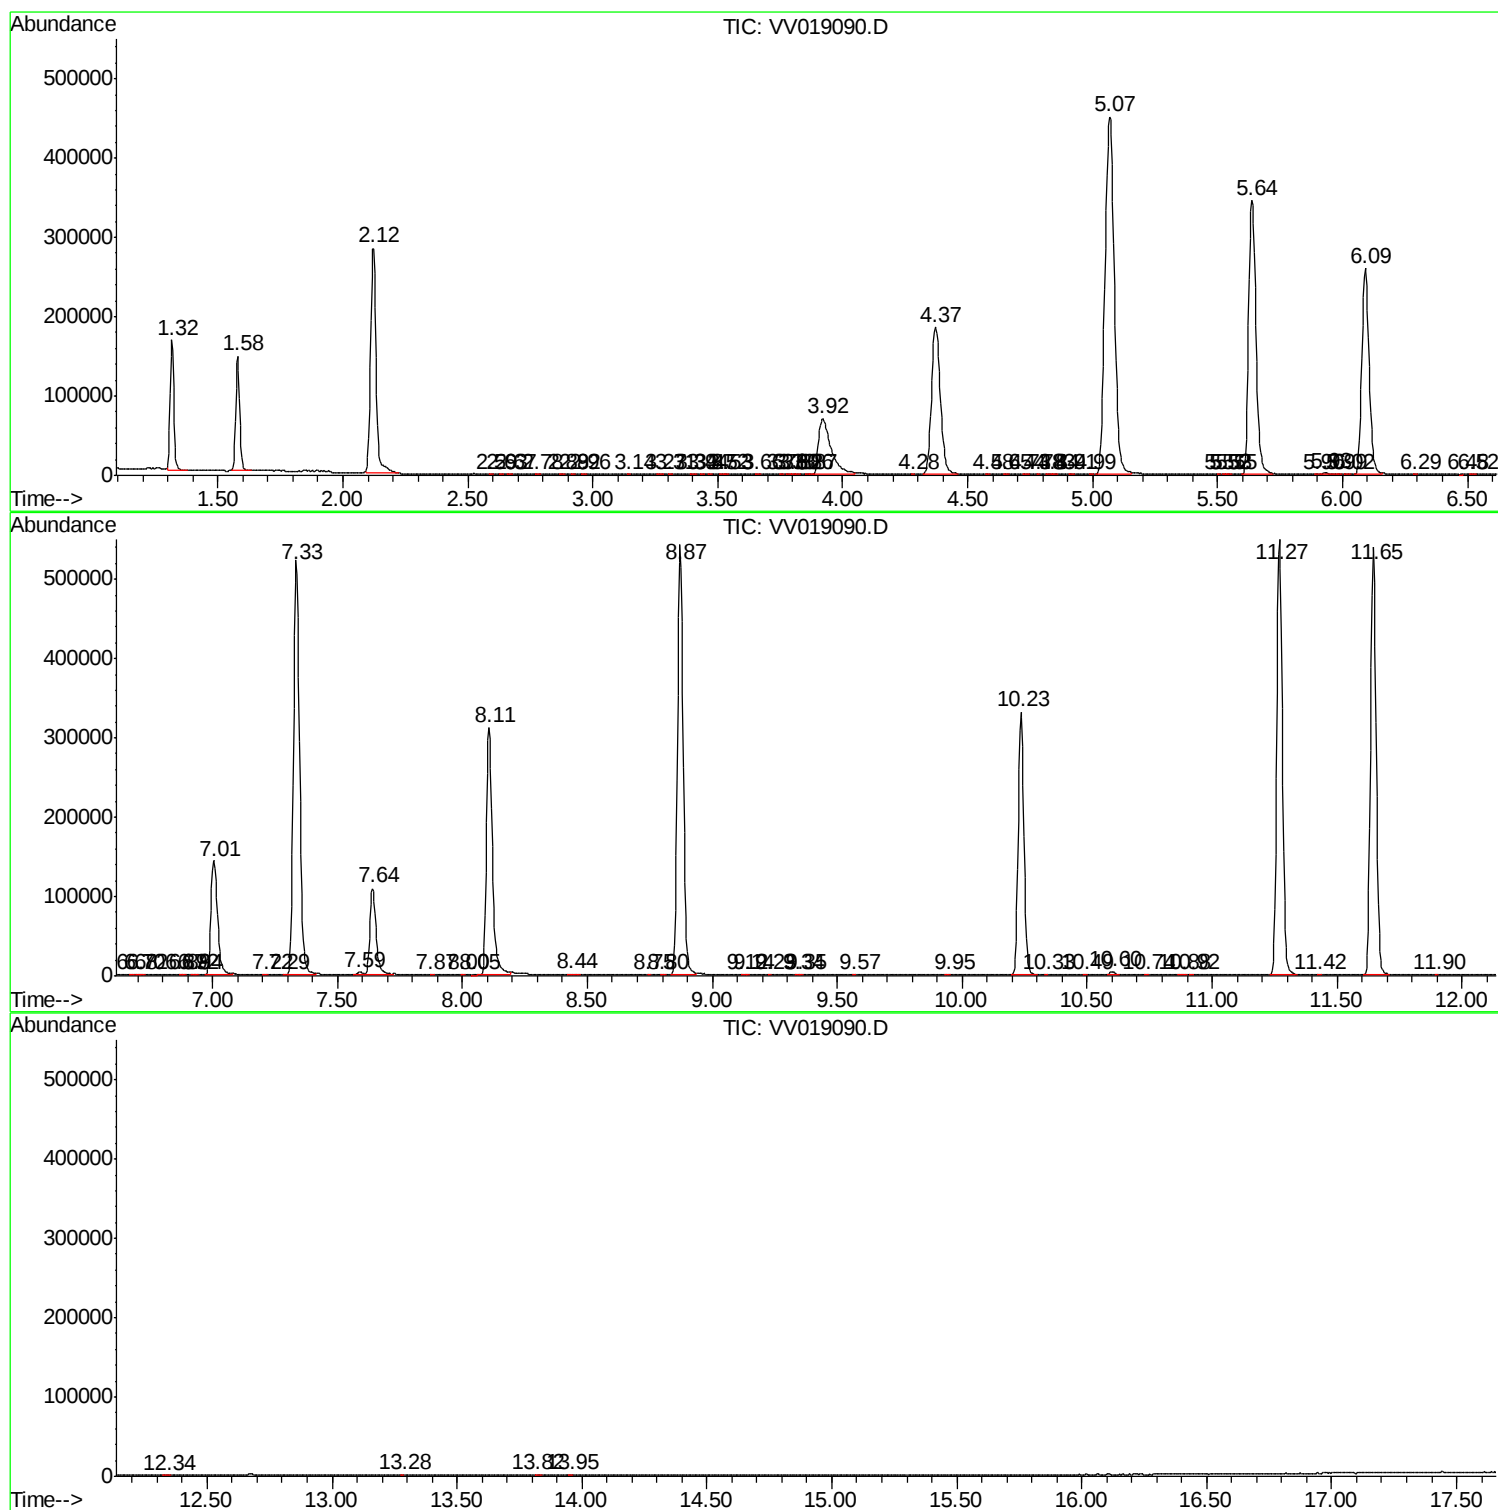

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102320\
Data File : VV019090.D
Acq On : 23 Oct 2020 14:26
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102320\
Data File : VV019090.D
Acq On : 23 Oct 2020 14:26
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc