

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019098.D
 Acq On : 23 Oct 2020 17:42
 Operator : SY/MD
 Sample : L4502-02ME 2X
 Misc : 5.82g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG436ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	89	rVB	178824	199006	14.64%	1.971%
2	1.579	145	152	166	rBV	135680	171139	12.59%	1.695%
3	2.113	307	318	328	rBV	343248	499990	36.78%	4.953%
4	2.389	401	404	408	rBV2	427	438	0.03%	0.004%
5	2.518	440	444	451	rBV3	1217	1521	0.11%	0.015%
6	2.634	471	480	491	rBV3	2458	4935	0.36%	0.049%
7	2.946	574	577	579	rBV	322	234	0.02%	0.002%
8	3.055	607	611	617	rBV2	364	310	0.02%	0.003%
9	3.081	617	619	621	rBV	220	122	0.01%	0.001%
10	3.151	637	641	644	rBV	305	180	0.01%	0.002%
11	3.177	647	649	651	rBV	262	145	0.01%	0.001%
12	3.274	677	679	680	rBV2	178	57	0.00%	0.001%
13	3.360	703	706	707	rBV	155	98	0.01%	0.001%
14	3.370	707	709	712	rVB2	297	132	0.01%	0.001%
15	3.483	741	744	746	rBV2	334	217	0.02%	0.002%
16	3.508	749	752	753	rBV	137	78	0.01%	0.001%
17	3.557	764	767	769	rBV3	311	222	0.02%	0.002%
18	3.669	800	802	803	rBV3	196	85	0.01%	0.001%
19	3.708	812	814	818	rVB	227	124	0.01%	0.001%
20	3.756	824	829	834	rBV	198	245	0.02%	0.002%
21	3.775	834	835	837	rBV	125	58	0.00%	0.001%
22	3.846	854	857	861	rVB	278	218	0.02%	0.002%
23	3.872	861	865	867	rBV2	180	137	0.01%	0.001%
24	3.920	870	880	926	rBV	70790	258900	19.05%	2.565%
25	4.373	1005	1021	1051	rBV	216053	529962	38.99%	5.250%
26	4.782	1147	1148	1151	rBV2	190	107	0.01%	0.001%
27	4.872	1173	1176	1179	rBV3	415	343	0.03%	0.003%
28	4.946	1196	1199	1201	rBV	206	115	0.01%	0.001%
29	4.997	1214	1215	1216	rBV	150	40	0.00%	0.000%
30	5.068	1220	1237	1266	rBV2	544436	1359372	100.00%	13.466%
31	5.309	1310	1312	1315	rVB2	410	207	0.02%	0.002%
32	5.351	1322	1325	1328	rBV3	830	735	0.05%	0.007%
33	5.421	1345	1347	1350	rVB	371	166	0.01%	0.002%
34	5.438	1350	1352	1358	rBV3	552	437	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019098.D
 Acq On : 23 Oct 2020 17:42
 Operator : SY/MD
 Sample : L4502-02ME 2X
 Misc : 5.82g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG436ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

35	5.466	1358	1361	1363	rBV2	322	193	0.01%	0.002%
36	5.573	1391	1394	1397	rBV	222	157	0.01%	0.002%
37	5.640	1401	1415	1440	rBV	345438	692315	50.93%	6.858%
38	5.939	1498	1508	1522	rVB8	4483	8418	0.62%	0.083%
39	6.093	1542	1556	1582	rBV	299695	611254	44.97%	6.055%
40	6.280	1612	1614	1617	rVB3	500	214	0.02%	0.002%
41	6.347	1634	1635	1636	rVB3	112	22	0.00%	0.000%
42	6.364	1636	1640	1644	rBV	464	401	0.03%	0.004%
43	6.431	1659	1661	1663	rBV	154	73	0.01%	0.001%
44	6.470	1672	1673	1675	rVB	393	98	0.01%	0.001%
45	6.502	1681	1683	1686	rBV	362	223	0.02%	0.002%
46	6.624	1719	1721	1723	rBV	149	93	0.01%	0.001%
47	6.798	1768	1775	1780	rBV2	485	640	0.05%	0.006%
48	6.823	1780	1783	1785	rBV2	188	121	0.01%	0.001%
49	6.862	1792	1795	1800	rBV	371	257	0.02%	0.003%
50	6.933	1815	1817	1819	rBV	87	43	0.00%	0.000%
51	6.955	1822	1824	1828	rVB	197	115	0.01%	0.001%
52	7.007	1828	1840	1868	rBV	170488	314997	23.17%	3.120%
53	7.222	1905	1907	1909	rBV	309	217	0.02%	0.002%
54	7.277	1923	1924	1927	rVB	281	144	0.01%	0.001%
55	7.296	1927	1930	1931	rBV	629	283	0.02%	0.003%
56	7.335	1931	1942	1966	rBV	628346	1080179	79.46%	10.700%
57	7.640	2028	2037	2067	rBV	123635	222854	16.39%	2.208%
58	7.785	2080	2082	2085	rBV2	389	206	0.02%	0.002%
59	7.897	2111	2117	2119	rBV3	407	432	0.03%	0.004%
60	7.929	2124	2127	2129	rBV2	393	241	0.02%	0.002%
61	7.997	2137	2148	2164	rBV	66210	112127	8.25%	1.111%
62	8.119	2174	2186	2224	rBV2	222717	632100	46.50%	6.261%
63	8.662	2352	2355	2359	rBV2	380	283	0.02%	0.003%
64	8.804	2397	2399	2400	rBV2	174	78	0.01%	0.001%
65	8.875	2409	2421	2443	rBV	525889	871462	64.11%	8.633%
66	9.045	2470	2474	2480	rBV3	572	571	0.04%	0.006%
67	9.254	2535	2539	2544	rBV2	456	408	0.03%	0.004%
68	9.338	2563	2565	2567	rBV	172	89	0.01%	0.001%
69	9.351	2567	2569	2571	rBV	287	149	0.01%	0.001%
70	9.405	2583	2586	2590	rBV	418	265	0.02%	0.003%
71	9.518	2618	2621	2623	rBV	197	128	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019098.D
 Acq On : 23 Oct 2020 17:42
 Operator : SY/MD
 Sample : L4502-02ME 2X
 Misc : 5.82g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG436ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

72	9.576	2634	2639	2642	rBV	330	361	0.03%	0.004%
73	9.736	2684	2689	2694	rBV2	400	300	0.02%	0.003%
74	9.891	2733	2737	2740	rBV	339	274	0.02%	0.003%
75	10.000	2768	2771	2772	rBV	139	78	0.01%	0.001%
76	10.090	2796	2799	2802	rBV2	277	178	0.01%	0.002%
77	10.106	2802	2804	2805	rBV	218	77	0.01%	0.001%
78	10.241	2833	2846	2867	rBV	374290	613449	45.13%	6.077%
79	10.412	2896	2899	2901	rBV2	278	171	0.01%	0.002%
80	10.460	2911	2914	2917	rBV2	356	228	0.02%	0.002%
81	10.576	2945	2950	2951	rBV2	221	189	0.01%	0.002%
82	10.900	3041	3051	3053	rBV2	389	663	0.05%	0.007%
83	11.138	3121	3125	3126	rBV	183	141	0.01%	0.001%
84	11.273	3155	3167	3193	rBV	555285	862647	63.46%	8.545%
85	11.437	3216	3218	3220	rBV	330	110	0.01%	0.001%
86	11.450	3220	3222	3224	rVV3	312	115	0.01%	0.001%
87	11.502	3236	3238	3240	rBV	214	119	0.01%	0.001%
88	11.595	3264	3267	3269	rBV	273	179	0.01%	0.002%
89	11.649	3271	3284	3306	rVV	660723	1032607	75.96%	10.229%
90	11.881	3353	3356	3358	rBV	327	202	0.01%	0.002%
91	12.026	3397	3401	3404	rBV	455	368	0.03%	0.004%
92	12.379	3508	3511	3513	rBV	463	285	0.02%	0.003%
93	12.424	3521	3525	3528	rBV2	234	215	0.02%	0.002%
94	12.929	3680	3682	3683	rBV2	341	160	0.01%	0.002%


Sum of corrected areas: 10095041

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102320\
Data File : VV019098.D
Acq On : 23 Oct 2020 17:42
Operator : SY/MD
Sample : L4502-02ME 2X
Misc : 5.82g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG436ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

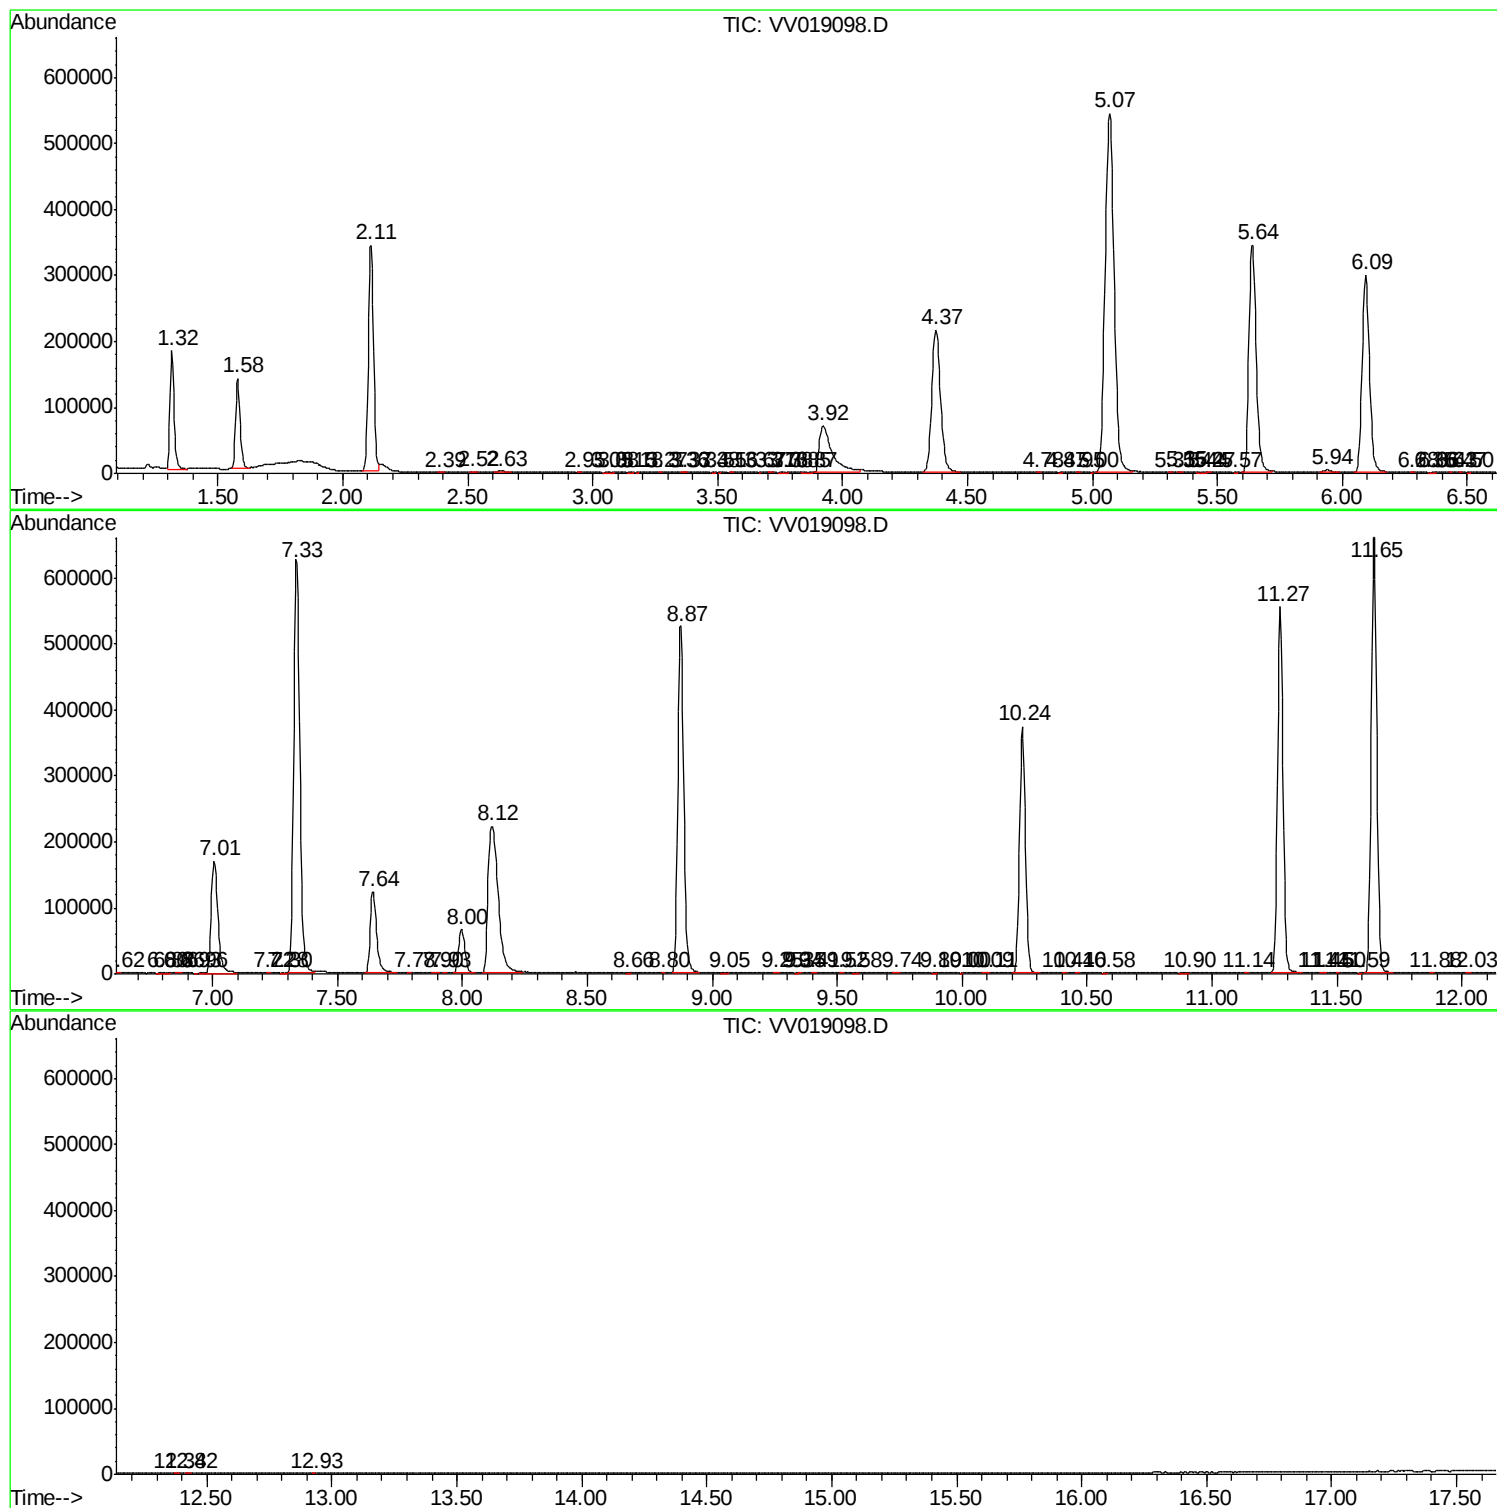

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102320\
Data File : VV019098.D
Acq On : 23 Oct 2020 17:42
Operator : SY/MD
Sample : L4502-02ME 2X
Misc : 5.82g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG436ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV102320\
Data File : VV019098.D
Acq On : 23 Oct 2020 17:42
Operator : SY/MD
Sample : L4502-02ME 2X
Misc : 5.82g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG436ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc