

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019100.D
 Acq On : 23 Oct 2020 18:30
 Operator : SY/MD
 Sample : L4502-01ME 2X
 Misc : 5.57g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG435ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	88	rVB	271889	299109	14.17%	1.806%
2	1.579	144	152	166	rVB	225172	274539	13.00%	1.658%
3	2.113	307	318	331	rBV	525571	764051	36.18%	4.614%
4	2.521	438	445	450	rBV4	1553	2129	0.10%	0.013%
5	2.592	464	467	469	rBV	433	257	0.01%	0.002%
6	2.637	469	481	492	rBV5	2798	5916	0.28%	0.036%
7	2.984	587	589	593	rVB2	413	317	0.02%	0.002%
8	3.061	609	613	618	rBV3	634	484	0.02%	0.003%
9	3.132	632	635	640	rVB2	383	345	0.02%	0.002%
10	3.396	712	717	721	rBV	303	351	0.02%	0.002%
11	3.428	723	727	732	rVB3	503	376	0.02%	0.002%
12	3.499	743	749	753	rBV2	252	251	0.01%	0.002%
13	3.524	753	757	761	rBV3	342	273	0.01%	0.002%
14	3.589	774	777	780	rBV	421	249	0.01%	0.002%
15	3.653	794	797	803	rVB2	361	283	0.01%	0.002%
16	3.798	839	842	848	rVB	246	241	0.01%	0.001%
17	3.840	848	855	860	rBV2	285	431	0.02%	0.003%
18	3.920	868	880	925	rBV	112847	418320	19.81%	2.526%
19	4.290	991	995	997	rBV3	477	435	0.02%	0.003%
20	4.370	1003	1020	1053	rBV	336956	818732	38.77%	4.944%
21	4.733	1129	1133	1135	rBV3	500	320	0.02%	0.002%
22	4.814	1156	1158	1162	rVV2	404	297	0.01%	0.002%
23	4.833	1162	1164	1168	rVB	491	278	0.01%	0.002%
24	4.872	1168	1176	1178	rBV2	441	441	0.02%	0.003%
25	4.888	1178	1181	1184	rVB2	347	271	0.01%	0.002%
26	5.000	1213	1216	1220	rVB2	317	282	0.01%	0.002%
27	5.068	1220	1237	1270	rBV2	844071	2111583	100.00%	12.750%
28	5.245	1291	1292	1299	rVB4	636	521	0.02%	0.003%
29	5.364	1325	1329	1331	rBV4	560	449	0.02%	0.003%
30	5.550	1381	1387	1391	rVB2	572	523	0.02%	0.003%
31	5.637	1401	1414	1440	rBV	585914	1152387	54.57%	6.958%
32	5.865	1484	1485	1491	rVB3	626	267	0.01%	0.002%
33	5.936	1496	1507	1524	rBV6	9135	20658	0.98%	0.125%
34	6.007	1524	1529	1532	rBV3	790	811	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019100.D
 Acq On : 23 Oct 2020 18:30
 Operator : SY/MD
 Sample : L4502-01ME 2X
 Misc : 5.57g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG435ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

35	6.090	1541	1555	1586	rBV	469519	943884	44.70%	5.699%
36	6.235	1593	1600	1611	rVB7	1263	2511	0.12%	0.015%
37	6.405	1648	1653	1661	rVV2	335	462	0.02%	0.003%
38	6.447	1663	1666	1670	rVB2	393	267	0.01%	0.002%
39	6.531	1689	1692	1697	rVB2	371	297	0.01%	0.002%
40	6.637	1715	1725	1727	rBV2	331	430	0.02%	0.003%
41	6.653	1727	1730	1733	rBV3	415	334	0.02%	0.002%
42	6.775	1764	1768	1775	rBV2	331	366	0.02%	0.002%
43	6.862	1788	1795	1797	rVB2	334	347	0.02%	0.002%
44	7.007	1828	1840	1870	rBV	274115	491861	23.29%	2.970%
45	7.274	1921	1923	1926	rVB2	570	329	0.02%	0.002%
46	7.335	1929	1942	1967	rBV	992884	1694088	80.23%	10.229%
47	7.640	2025	2037	2069	rBV	201560	351617	16.65%	2.123%
48	7.814	2089	2091	2098	rVB3	904	651	0.03%	0.004%
49	7.994	2135	2147	2168	rBV	376475	637032	30.17%	3.847%
50	8.116	2173	2185	2222	rBV	378443	1018931	48.25%	6.153%
51	8.454	2286	2290	2300	rVB5	1880	2769	0.13%	0.017%
52	8.617	2338	2341	2345	rBV	302	274	0.01%	0.002%
53	8.871	2408	2420	2453	rBV	875190	1449923	68.67%	8.755%
54	9.052	2473	2476	2479	rVB2	320	238	0.01%	0.001%
55	9.135	2500	2502	2510	rVB4	527	460	0.02%	0.003%
56	9.180	2510	2516	2521	rBV4	446	467	0.02%	0.003%
57	9.228	2524	2531	2535	rBV2	435	441	0.02%	0.003%
58	9.283	2544	2548	2551	rBV3	451	322	0.02%	0.002%
59	9.354	2567	2570	2573	rVB	419	267	0.01%	0.002%
60	9.486	2607	2611	2613	rBV	408	250	0.01%	0.002%
61	9.621	2650	2653	2656	rBV	276	248	0.01%	0.001%
62	9.653	2661	2663	2670	rVB2	360	327	0.02%	0.002%
63	9.733	2683	2688	2691	rBV3	313	335	0.02%	0.002%
64	9.836	2715	2720	2721	rBV2	299	275	0.01%	0.002%
65	9.968	2759	2761	2765	rVV	290	263	0.01%	0.002%
66	10.039	2779	2783	2786	rVB2	329	247	0.01%	0.001%
67	10.061	2786	2790	2793	rBV3	373	311	0.01%	0.002%
68	10.241	2832	2846	2866	rBV	586644	964849	45.69%	5.826%
69	10.434	2903	2906	2913	rBV3	352	373	0.02%	0.002%
70	10.537	2929	2938	2940	rBV2	313	429	0.02%	0.003%
71	10.595	2952	2956	2963	rBV5	548	765	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019100.D
 Acq On : 23 Oct 2020 18:30
 Operator : SY/MD
 Sample : L4502-01ME 2X
 Misc : 5.57g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG435ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

72	10.666	2974	2978	2982	rVB3	345	320	0.02%	0.002%
73	10.881	3039	3045	3050	rBV5	1045	1019	0.05%	0.006%
74	11.193	3138	3142	3147	rVV4	404	465	0.02%	0.003%
75	11.270	3155	3166	3188	rBV	969346	1469950	69.61%	8.876%
76	11.646	3267	3283	3309	rBV	1048692	1635610	77.46%	9.876%
77	12.145	3435	3438	3439	rBV	442	252	0.01%	0.002%
78	12.225	3459	3463	3467	rBV	219	239	0.01%	0.001%
79	12.273	3473	3478	3480	rBV3	488	425	0.02%	0.003%
80	12.473	3537	3540	3543	rBV2	510	380	0.02%	0.002%
81	12.486	3543	3544	3547	rVV2	489	263	0.01%	0.002%
82	12.527	3551	3557	3561	rVV2	514	587	0.03%	0.004%
83	12.875	3663	3665	3672	rVB2	317	323	0.02%	0.002%
84	13.010	3704	3707	3709	rBV2	346	241	0.01%	0.001%
85	13.067	3721	3725	3728	rBV2	385	321	0.02%	0.002%
86	13.537	3869	3871	3876	rVB3	352	273	0.01%	0.002%
87	13.884	3975	3979	3984	rBV	441	418	0.02%	0.003%
88	13.916	3984	3989	3992	rBV2	563	568	0.03%	0.003%
89	14.058	4031	4033	4038	rVV3	301	254	0.01%	0.002%
90	14.119	4044	4052	4055	rBV3	436	597	0.03%	0.004%
91	14.177	4066	4070	4077	rBV3	411	515	0.02%	0.003%
92	14.460	4156	4158	4165	rBV3	336	385	0.02%	0.002%
93	14.704	4231	4234	4238	rBV2	454	427	0.02%	0.003%
94	14.775	4253	4256	4258	rBV2	439	244	0.01%	0.001%
95	14.807	4264	4266	4270	rBV2	473	324	0.02%	0.002%
96	15.839	4581	4587	4589	rBV4	746	729	0.03%	0.004%
97	15.919	4608	4612	4617	rBV3	919	903	0.04%	0.005%
98	16.048	4649	4652	4656	rBV3	707	680	0.03%	0.004%
99	16.071	4657	4659	4662	rVV3	635	364	0.02%	0.002%
100	16.411	4762	4765	4767	rBV4	662	370	0.02%	0.002%


Sum of corrected areas: 16560863

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102320\
Data File : VV019100.D
Acq On : 23 Oct 2020 18:30
Operator : SY/MD
Sample : L4502-01ME 2X
Misc : 5.57g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG435ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

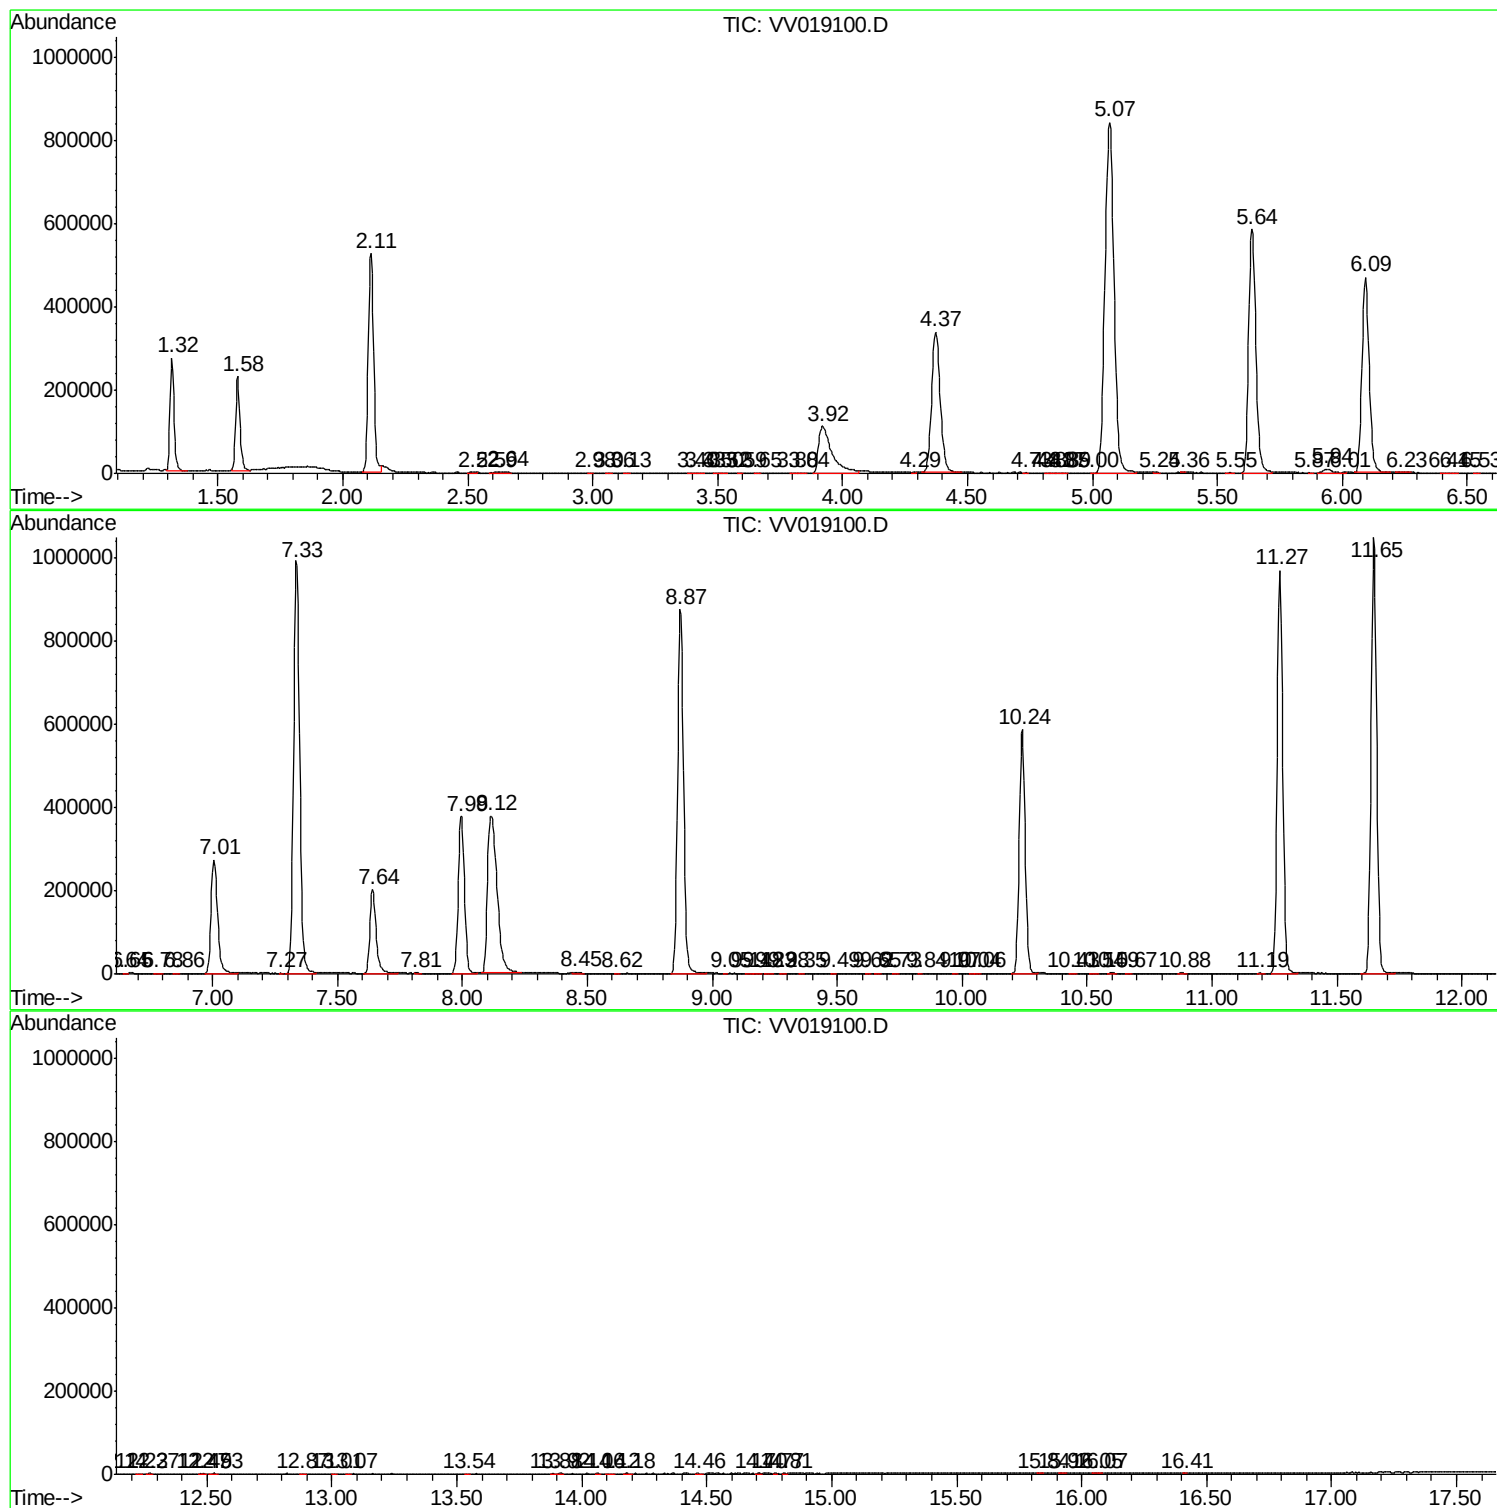

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV102320\
Data File : VV019100.D
Acq On : 23 Oct 2020 18:30
Operator : SY/MD
Sample : L4502-01ME 2X
Misc : 5.57g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG435ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102320\
Data File : VV019100.D
Acq On : 23 Oct 2020 18:30
Operator : SY/MD
Sample : L4502-01ME 2X
Misc : 5.57g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG435ME

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc