

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019105.D
 Acq On : 23 Oct 2020 20:28
 Operator : SY/MD
 Sample : L4471-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	181527	174160	14.80%	1.973%
2	1.579	145	152	167	rVB	148269	165595	14.07%	1.876%
3	2.122	312	321	353	rVB	298528	456509	38.78%	5.171%
4	2.357	391	394	397	rBV2	297	198	0.02%	0.002%
5	2.399	403	407	412	rBV2	538	539	0.05%	0.006%
6	2.454	422	424	425	rBV	334	126	0.01%	0.001%
7	2.573	459	461	464	rBV	266	170	0.01%	0.002%
8	2.685	493	496	502	rBB3	285	219	0.02%	0.002%
9	2.746	512	515	517	rBV	415	192	0.02%	0.002%
10	2.814	533	536	537	rBV	334	149	0.01%	0.002%
11	2.920	566	569	572	rBV2	201	173	0.01%	0.002%
12	3.016	596	599	601	rBV2	165	126	0.01%	0.001%
13	3.106	624	627	629	rBV	299	154	0.01%	0.002%
14	3.132	629	635	637	rBV2	216	207	0.02%	0.002%
15	3.306	687	689	695	rVB2	328	215	0.02%	0.002%
16	3.386	707	714	715	rBV	300	222	0.02%	0.003%
17	3.473	739	741	743	rBV	159	97	0.01%	0.001%
18	3.592	772	778	779	rBV2	165	171	0.01%	0.002%
19	3.666	798	801	804	rBV2	251	212	0.02%	0.002%
20	3.698	808	811	816	rVV	222	180	0.02%	0.002%
21	3.807	839	845	846	rBV2	309	215	0.02%	0.002%
22	3.833	851	853	857	rVV2	289	188	0.02%	0.002%
23	3.917	868	879	918	rBV2	75000	236237	20.07%	2.676%
24	4.376	1006	1022	1046	rBV	189477	463595	39.38%	5.251%
25	4.724	1128	1130	1134	rVB	260	140	0.01%	0.002%
26	4.746	1134	1137	1140	rBV3	365	218	0.02%	0.002%
27	4.781	1145	1148	1150	rBV2	146	64	0.01%	0.001%
28	4.804	1153	1155	1157	rBV2	419	248	0.02%	0.003%
29	4.830	1161	1163	1165	rBV2	147	88	0.01%	0.001%
30	4.875	1171	1177	1179	rBV2	364	329	0.03%	0.004%
31	4.955	1199	1202	1206	rBV2	450	359	0.03%	0.004%
32	4.984	1206	1211	1213	rVV4	381	295	0.03%	0.003%
33	5.071	1221	1238	1274	rBV2	458976	1177109	100.00%	13.333%
34	5.425	1346	1348	1351	rBV3	160	121	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019105.D
 Acq On : 23 Oct 2020 20:28
 Operator : SY/MD
 Sample : L4471-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

35	5.482	1362	1366	1374	rVB3	585	596	0.05%	0.007%
36	5.518	1374	1377	1378	rBV3	253	135	0.01%	0.002%
37	5.579	1393	1396	1399	rBV2	105	62	0.01%	0.001%
38	5.595	1399	1401	1402	rBV	155	68	0.01%	0.001%
39	5.640	1403	1415	1441	rBV	344801	684401	58.14%	7.752%
40	5.933	1500	1506	1520	rBV4	2157	3589	0.30%	0.041%
41	6.016	1530	1532	1535	rVB	350	185	0.02%	0.002%
42	6.035	1535	1538	1542	rBV2	314	257	0.02%	0.003%
43	6.093	1542	1556	1590	rBV	265049	532834	45.27%	6.035%
44	6.328	1625	1629	1631	rBV3	442	271	0.02%	0.003%
45	6.457	1667	1669	1672	rBV	224	138	0.01%	0.002%
46	6.540	1691	1695	1698	rBV	358	317	0.03%	0.004%
47	6.617	1717	1719	1720	rBV	217	79	0.01%	0.001%
48	6.662	1730	1733	1736	rBV2	176	112	0.01%	0.001%
49	6.855	1791	1793	1797	rVB2	243	164	0.01%	0.002%
50	6.875	1797	1799	1805	rVB2	252	209	0.02%	0.002%
51	6.907	1805	1809	1815	rBV2	311	311	0.03%	0.004%
52	6.945	1815	1821	1822	rBV	291	246	0.02%	0.003%
53	7.006	1830	1840	1864	rBV2	144076	264831	22.50%	3.000%
54	7.215	1902	1905	1906	rBV3	329	163	0.01%	0.002%
55	7.289	1926	1928	1931	rVB	374	135	0.01%	0.002%
56	7.338	1931	1943	1970	rBV	538491	920577	78.21%	10.427%
57	7.518	1997	1999	2004	rBV3	521	318	0.03%	0.004%
58	7.604	2023	2026	2027	rBV	204	109	0.01%	0.001%
59	7.643	2027	2038	2063	rVV	107603	186553	15.85%	2.113%
60	7.887	2111	2114	2117	rBV2	272	193	0.02%	0.002%
61	8.058	2163	2167	2170	rBV2	283	230	0.02%	0.003%
62	8.106	2172	2182	2204	rBV	308661	515514	43.79%	5.839%
63	8.444	2279	2287	2292	rBV5	1245	1956	0.17%	0.022%
64	8.492	2299	2302	2306	rBV3	329	201	0.02%	0.002%
65	8.579	2326	2329	2334	rVB2	351	253	0.02%	0.003%
66	8.678	2355	2360	2363	rBV3	316	325	0.03%	0.004%
67	8.701	2365	2367	2371	rVV2	329	202	0.02%	0.002%
68	8.817	2399	2403	2404	rBV	319	214	0.02%	0.002%
69	8.871	2409	2420	2443	rBV	531244	859525	73.02%	9.736%
70	9.074	2480	2483	2485	rBV2	387	234	0.02%	0.003%
71	9.296	2549	2552	2553	rBV	203	109	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102320\
 Data File : VV019105.D
 Acq On : 23 Oct 2020 20:28
 Operator : SY/MD
 Sample : L4471-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

72	9.543	2628	2629	2630	rBV	132	33	0.00%	0.000%
73	9.627	2652	2655	2657	rBV	167	106	0.01%	0.001%
74	9.701	2675	2678	2681	rBV3	263	210	0.02%	0.002%
75	9.733	2686	2688	2689	rBV3	179	54	0.00%	0.001%
76	9.768	2694	2699	2705	rBV2	365	426	0.04%	0.005%
77	9.810	2710	2712	2716	rBV	216	107	0.01%	0.001%
78	9.910	2741	2743	2748	rVB2	182	79	0.01%	0.001%
79	9.939	2748	2752	2756	rBV2	297	257	0.02%	0.003%
80	10.235	2833	2844	2862	rBV	330214	520918	44.25%	5.900%
81	10.363	2882	2884	2886	rBV	383	197	0.02%	0.002%
82	10.460	2912	2914	2915	rBV2	176	58	0.00%	0.001%
83	10.473	2915	2918	2921	rVV	235	168	0.01%	0.002%
84	10.563	2944	2946	2950	rBV2	270	154	0.01%	0.002%
85	10.601	2956	2958	2962	rBV2	462	292	0.02%	0.003%
86	10.784	3012	3015	3018	rVB	312	170	0.01%	0.002%
87	10.907	3051	3053	3057	rBV	264	184	0.02%	0.002%
88	11.083	3106	3108	3111	rVB2	359	190	0.02%	0.002%
89	11.116	3111	3118	3124	rBV	420	619	0.05%	0.007%
90	11.270	3155	3166	3189	rBV	521104	799890	67.95%	9.060%
91	11.646	3270	3283	3305	rBV	533189	849112	72.14%	9.618%
92	12.405	3515	3519	3522	rBV	575	513	0.04%	0.006%
93	13.228	3772	3775	3778	rBV2	665	457	0.04%	0.005%




Sum of corrected areas: 8828630

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102320\
Data File : VV019105.D
Acq On : 23 Oct 2020 20:28
Operator : SY/MD
Sample : L4471-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

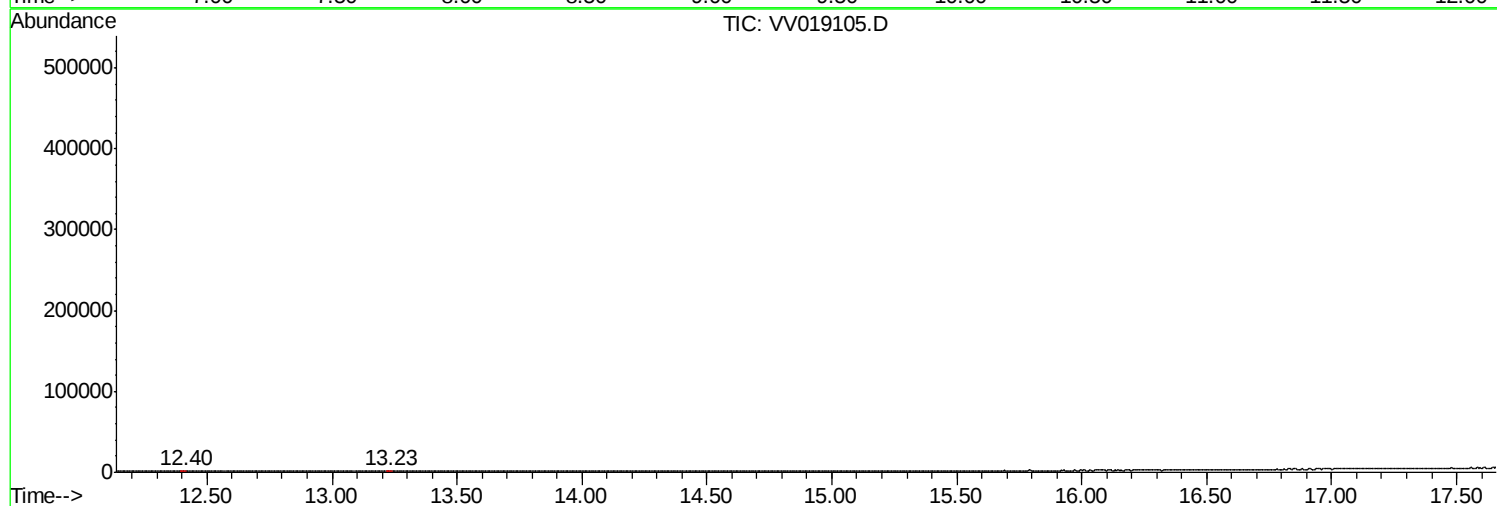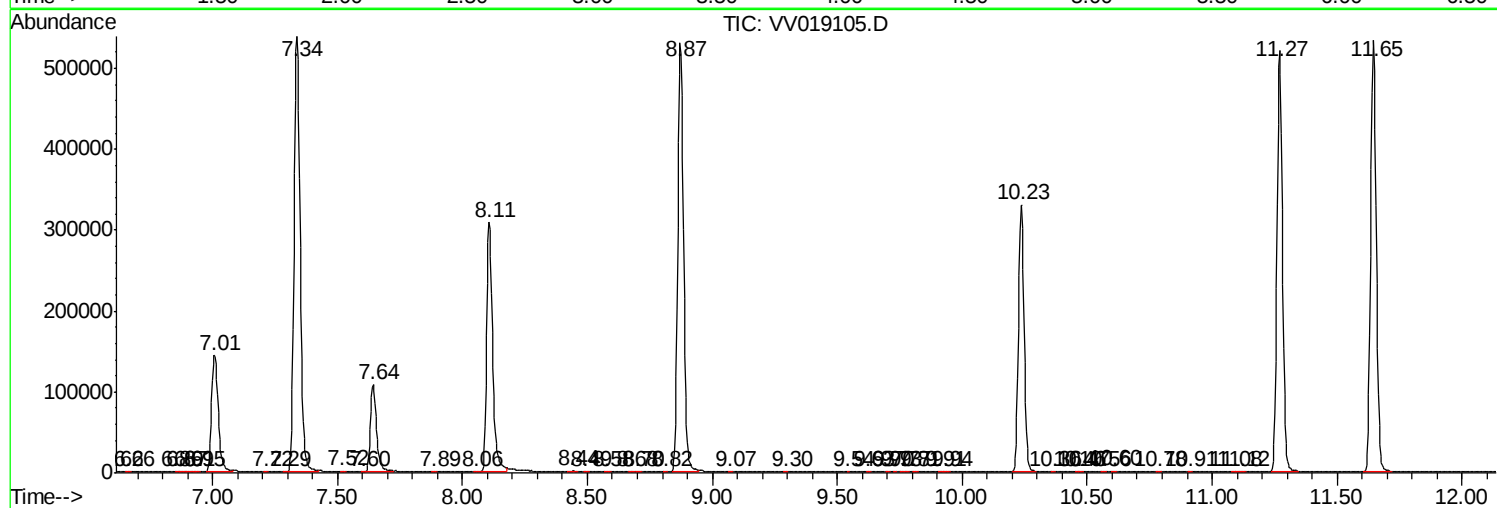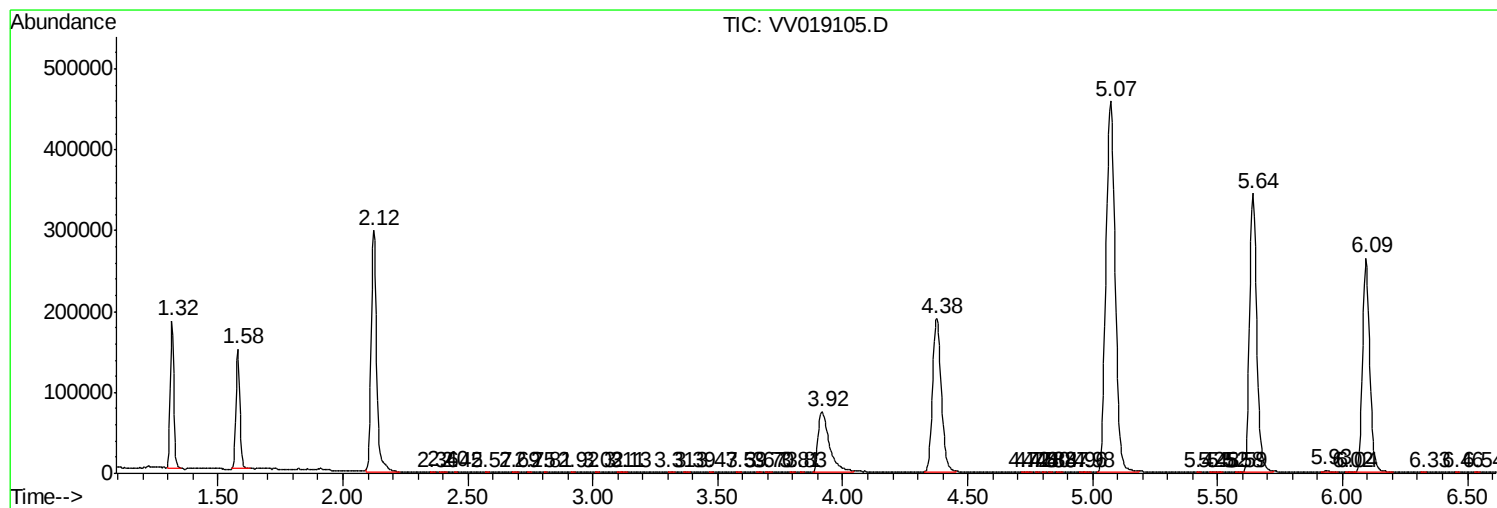

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102320\
Data File : VV019105.D
Acq On : 23 Oct 2020 20:28
Operator : SY/MD
Sample : L4471-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102320\
Data File : VV019105.D
Acq On : 23 Oct 2020 20:28
Operator : SY/MD
Sample : L4471-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc