


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV102320\
Data File : VV019085.D
Acq On : 23 Oct 2020 09:36
Operator : SY/MD
Sample : BFB81
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB81

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Title : VOC Analysis
Last Update : Thu Oct 29 03:08:29 2020

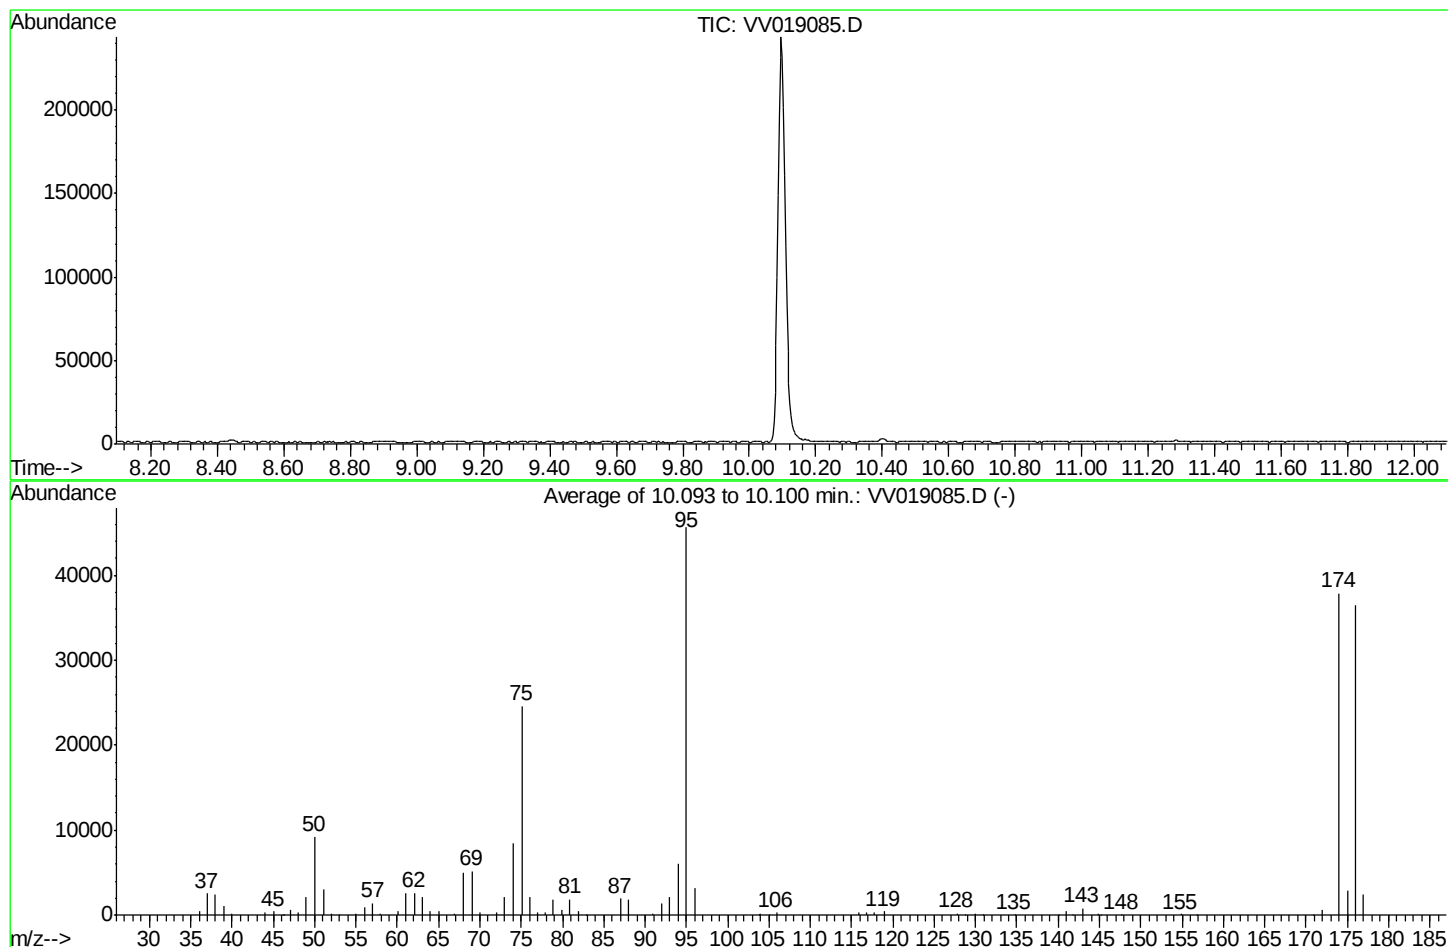

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	9262	PASS
75	95	30	80	54.0	24645	PASS
95	95	100	100	100.0	45666	PASS
96	95	5	9	6.9	3165	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.0	37880	PASS
175	174	5	9	7.7	2934	PASS
176	174	95	101	96.3	36480	PASS
177	176	5	9	6.7	2434	PASS

m/z	Abundance
.00	8.0
7.00	2400.0
8.00	2 1.0
9.00	1182.0
40.00	400.0
44.00	1224.0
45.00	4 .0
4 .10	128.0
47.10	512.0
48.00	20.0
49.00	2155.0
50.00	9085.0
51.00	29 9.0
52.10	14 .0
5 .00	121.0
54.90	217.0
5 .00	8 .0
57.00	1445.0
58.00	109.0
0.10	4 8.0
1.00	2 7 .0
2.10	2 8 .0
.00	1980.0
4.00	484.0
5.00	489.0
.90	1 2.0
8.00	4989.0
9.00	51 .0
70.00	.0
72.10	11.0
7 .00	222 .0
74.00	8 20.0
75.10	2 952.0
7 .00	2122.0
77.00	279.0
77.80	279.0
78.90	1792.0
79.90	05.0
80.90	1801.0
81.90	471.0
87.00	195 .0
88.00	18 9.0
90.90	182.0
92.00	12 4.0
9 .00	19 .0
94.00	19 .0
95.00	45 00.0
9 .10	129.0
10 .80	217.0
105.10	119.0
105.90	2 8.0
115.90	285.0
11 .80	295.0
117.80	2 .0
118.90	88.0
127.80	170.0
129.90	1 8.0
1 0.90	10 .0
140.90	51 .0
141.70	10 .0
14 .00	810.0
144.90	1 7.0
154.80	1 2.0
171.90	08.0
174.00	52.0
175.00	2977.0
17 .00	509 .0
177.00	2 8 .0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
.00	507.0
7.00	25 5.0
8.00	25 4.0
9.00	1171.0
40.00	400.0
44.00	1242.0
45.00	459.0
47.00	570.0
48.00	05.0
49.00	2229.0
50.00	9477.0
51.00	212.0
52.10	1 2.0
52.90	109.0
54.90	190.0
5 .00	887.0
57.10	1411.0
57.90	114.0
0.00	4 .0
1.00	2 07.0
2.00	2 58.0
.00	2191.0
4.00	487.0
5.00	48 .0
.90	1 .0
8.10	5227.0
9.00	5 41.0
70.00	5 .0
72.00	287.0
7 .00	2242.0
74.00	8 71.0
75.10	25504.0
7 .00	2159.0
7 .90	2 5.0
77.90	2 7.0
78.90	1922.0
79.90	4 .0
80.90	19 5.0
81.90	520.0
87.00	2005.0
88.00	1895.0
90.80	195.0
92.00	1 01.0
9 .00	218 .0
94.00	2 9.0
95.00	47208.0
9 .00	284.0
104.00	240.0
105.00	111.0
105.90	272.0
115.80	12.0
11 .80	29 .0
117.80	27 .0
118.90	425.0
127.80	215.0
129.90	194.0
1 4.70	109.0
140.90	5 .0
142.90	808.0
144.80	188.0
147.70	104.0
154.80	141.0
15 .80	101.0
171.90	95.0
174.00	9272.0
175.00	005.0
17 .00	7784.0
177.00	25 .0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
.00	427.0
7.00	2544.0
8.00	2444.0
9.00	105 .0
9.90	47.0
44.00	1185.0
45.00	98.0
4 . 0	128.0
47.00	58 .0
48.00	281.0
49.00	210 .0
50.00	9225.0
51.10	024.0
52.00	178.0
54.90	1 2.0
5 .00	805.0
57.10	1290.0
57.90	10 .0
0.00	459.0
1.00	2 81.0
2.00	2 94.0
.00	2222.0
4.00	4 .0
5.10	488.0
7.00	15 .0
8.10	4805.0
9.00	49 5.0
70.00	1 .0
72.00	252.0
7 .00	200 .0
74.00	8199.0
75.10	24480.0
7 .00	19 0.0
77.00	202.0
77.90	22 .0
78.90	1820.0
79.90	2.0
80.90	18 9.0
81.90	499.0
82.90	104.0
87.00	1909.0
88.00	1857.0
90.80	187.0
92.00	1 00.0
9 .00	2182.0
94.00	5 2.0
95.00	44192.0
9 .00	084.0
104.00	2 .0
105.90	258.0
115.90	1 .0
11 .90	29 .0
117.80	244.0
118.90	.0
127.80	240.0
128.80	115.0
129.90	198.0
1 4.70	105.0
140.00	107.0
140.90	50 .0
142.90	8 .0
144.70	207.0
145.10	1 .0
147.70	11 .0
154.90	1 .0
170.90	109.0
171.90	9 .0
174.00	801 .0
175.00	2822.0
17 .00	5 0.0
177.00	2 8 .0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

Scan 2789 (10.058 min): VV019085.D
BFB81

m/z	Abundance
40.00	245.0
44.00	920.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81