

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023006.D
 Acq On : 23 Oct 2021 13:26
 Operator : SY/MD
 Sample : VV1023WBL03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK234

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.089	11	15	26	rVB	10575	11861	2.36%	0.316%
2	1.298	74	80	91	rVB	76697	77662	15.45%	2.070%
3	1.561	154	162	178	rVB	63328	76965	15.32%	2.052%
4	2.101	320	330	344	rVB	96567	135655	26.99%	3.616%
5	2.503	444	455	466	rBV4	4525	8149	1.62%	0.217%
6	3.970	887	911	932	rBV2	36185	168933	33.62%	4.503%
7	4.346	1010	1028	1044	rBV	82635	203771	40.55%	5.432%
8	5.040	1228	1244	1281	rVB2	219581	502546	100.00%	13.396%
9	5.616	1410	1423	1443	rBV	146876	297119	59.12%	7.920%
10	5.899	1502	1511	1522	rVB6	4998	8459	1.68%	0.225%
11	6.072	1550	1565	1587	rBV	112773	233098	46.38%	6.213%
12	6.989	1838	1850	1871	rBV2	48775	94456	18.80%	2.518%
13	7.313	1938	1951	1969	rBV	200590	357543	71.15%	9.531%
14	7.625	2039	2048	2069	rBV2	29994	57889	11.52%	1.543%
15	8.108	2185	2198	2234	rBV2	194949	428640	85.29%	11.426%
16	8.854	2419	2430	2455	rBV	222449	366377	72.90%	9.766%
17	10.220	2843	2855	2866	rBV	78263	123480	24.57%	3.291%
18	11.249	3165	3175	3194	rBV	193747	300849	59.86%	8.019%
19	11.625	3281	3292	3310	rBV	188325	298044	59.31%	7.945%




Sum of corrected areas: 3751496

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023006.D
Acq On : 23 Oct 2021 13:26
Operator : SY/MD
Sample : VV1023WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK234

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

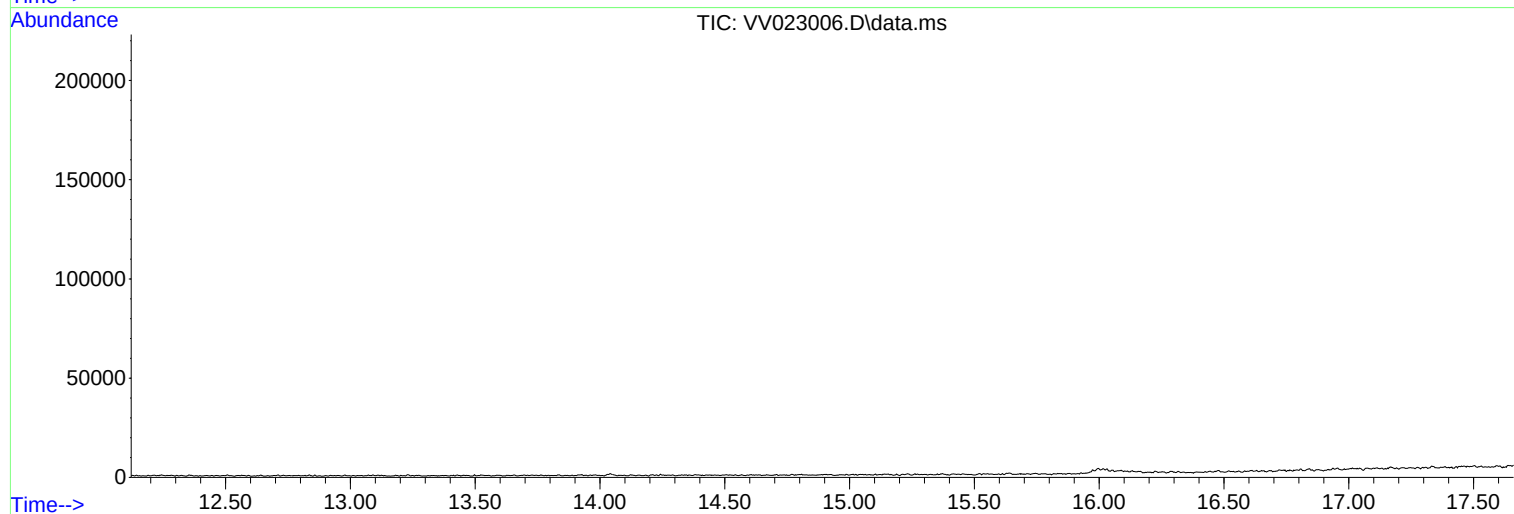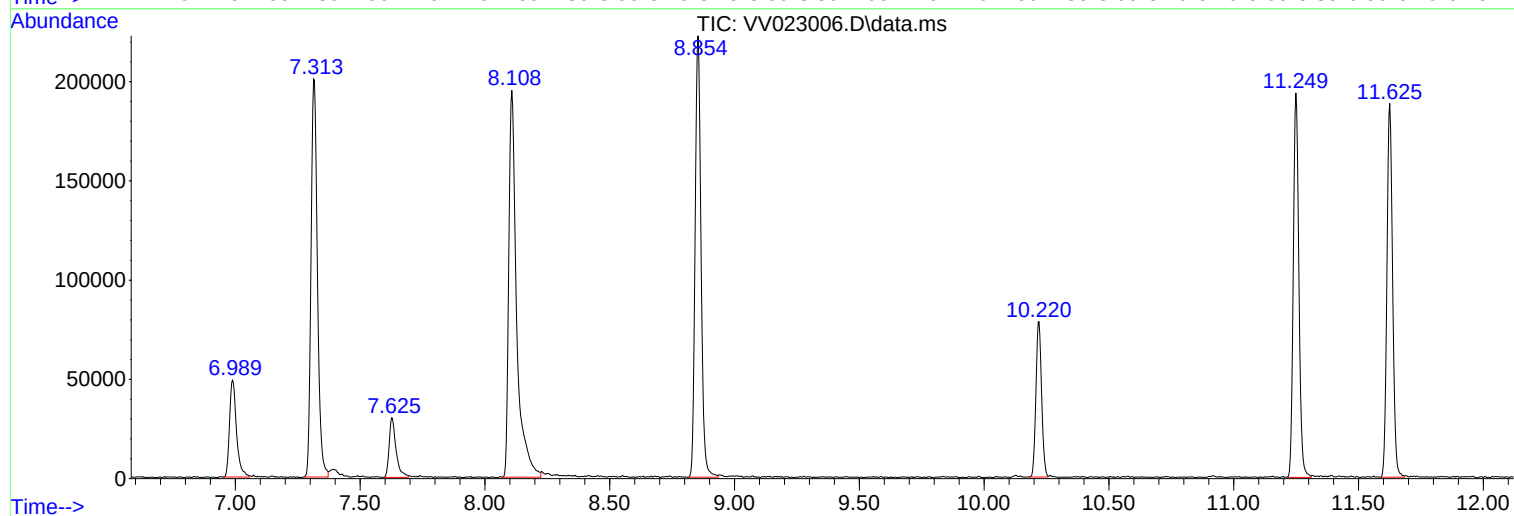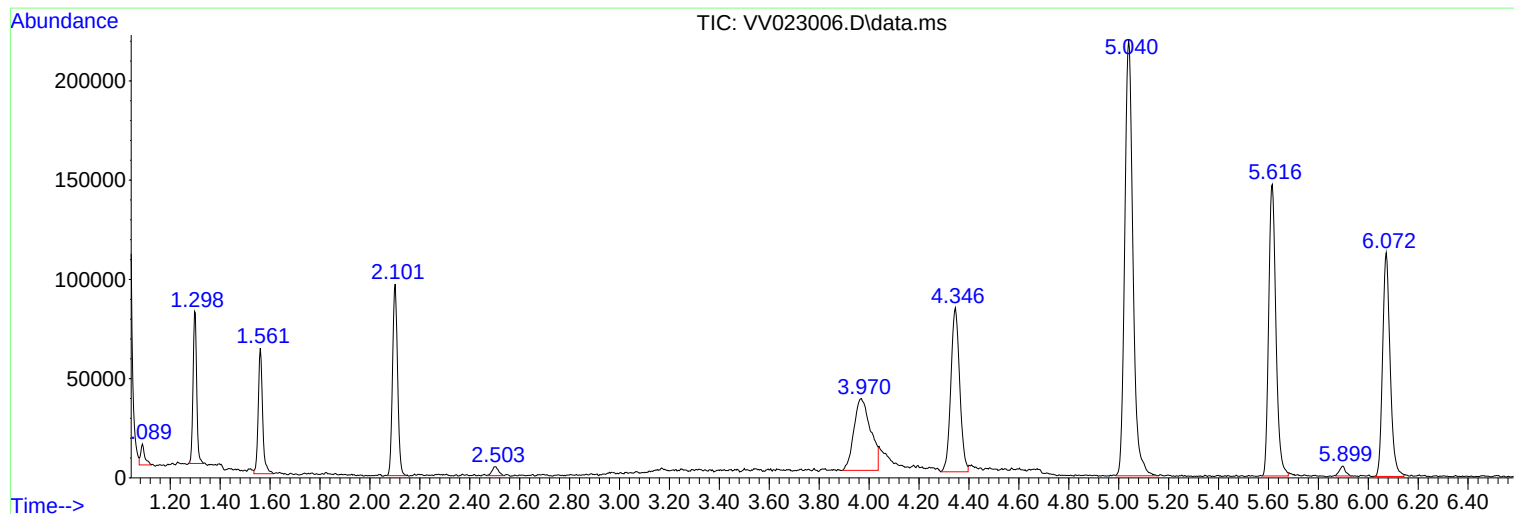

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023006.D
Acq On : 23 Oct 2021 13:26
Operator : SY/MD
Sample : VV1023WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK234

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023006.D
Acq On : 23 Oct 2021 13:26
Operator : SY/MD
Sample : VV1023WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK234

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------