

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023007.D
 Acq On : 23 Oct 2021 14:11
 Operator : SY/MD
 Sample : M4277-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG88

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023007.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	97488	99654	19.54%	2.373%
2	1.433	117	122	134	rVB	10831	11941	2.34%	0.284%
3	1.564	155	163	179	rVB2	66369	82531	16.18%	1.966%
4	2.105	319	331	344	rBV	125331	184525	36.18%	4.395%
5	2.185	346	356	376	rBV	9275	29544	5.79%	0.704%
6	3.905	875	891	928	rBV2	132603	387250	75.93%	9.223%
7	4.342	1010	1027	1047	rBV	92943	225400	44.20%	5.368%
8	5.040	1228	1244	1270	rBV2	210611	509987	100.00%	12.146%
9	5.612	1409	1422	1442	rBV	134187	273308	53.59%	6.509%
10	5.915	1503	1516	1529	rBV7	6953	15765	3.09%	0.375%
11	6.066	1550	1563	1582	rBV2	116726	239503	46.96%	5.704%
12	6.985	1839	1849	1866	rBV	47082	88825	17.42%	2.116%
13	7.313	1938	1951	1968	rBV	222747	389528	76.38%	9.277%
14	7.394	1968	1976	1985	rVB2	7751	13929	2.73%	0.332%
15	7.622	2036	2047	2064	rBV	29893	54271	10.64%	1.293%
16	7.976	2148	2157	2167	rVB3	9927	17198	3.37%	0.410%
17	8.095	2183	2194	2231	rBV2	173102	435493	85.39%	10.372%
18	8.850	2417	2429	2452	rBV	214055	357645	70.13%	8.518%
19	9.143	2510	2520	2534	rVB7	3863	7493	1.47%	0.178%
20	9.863	2735	2744	2750	rBV6	5459	8961	1.76%	0.213%
21	10.217	2843	2854	2867	rBV2	82788	130943	25.68%	3.119%
22	11.249	3164	3175	3194	rVB	189851	297584	58.35%	7.088%
23	11.535	3255	3264	3275	rBV7	3573	6257	1.23%	0.149%
24	11.625	3280	3292	3308	rBV	206538	331160	64.93%	7.887%




Sum of corrected areas: 4198695

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023007.D
Acq On : 23 Oct 2021 14:11
Operator : SY/MD
Sample : M4277-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

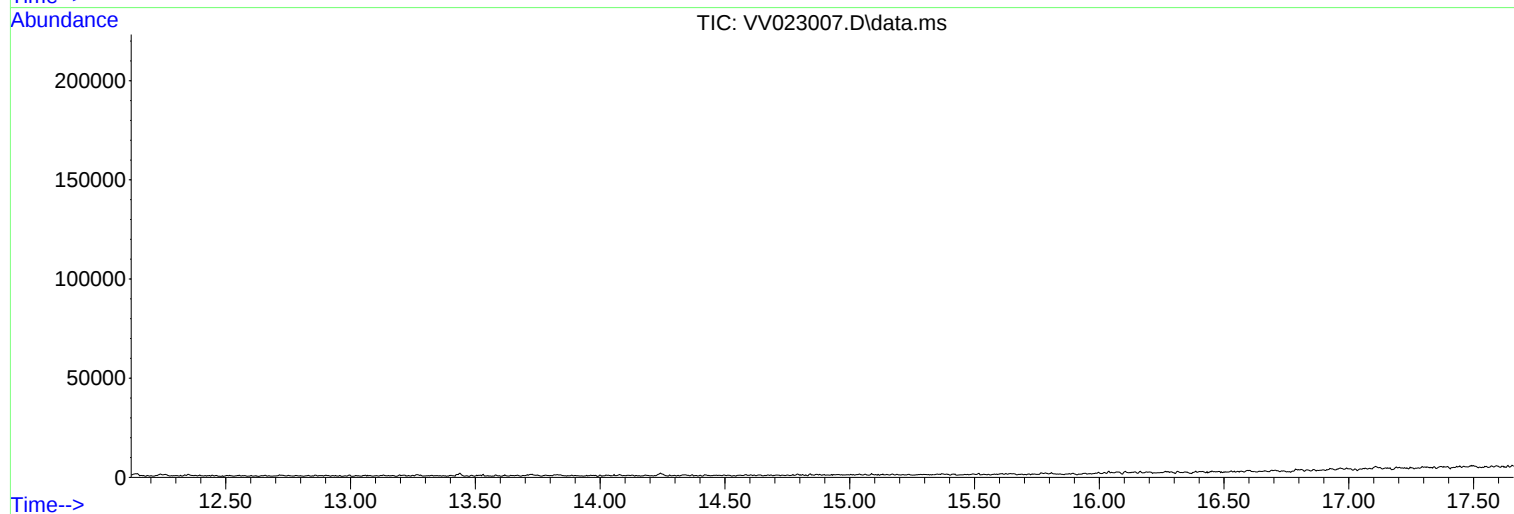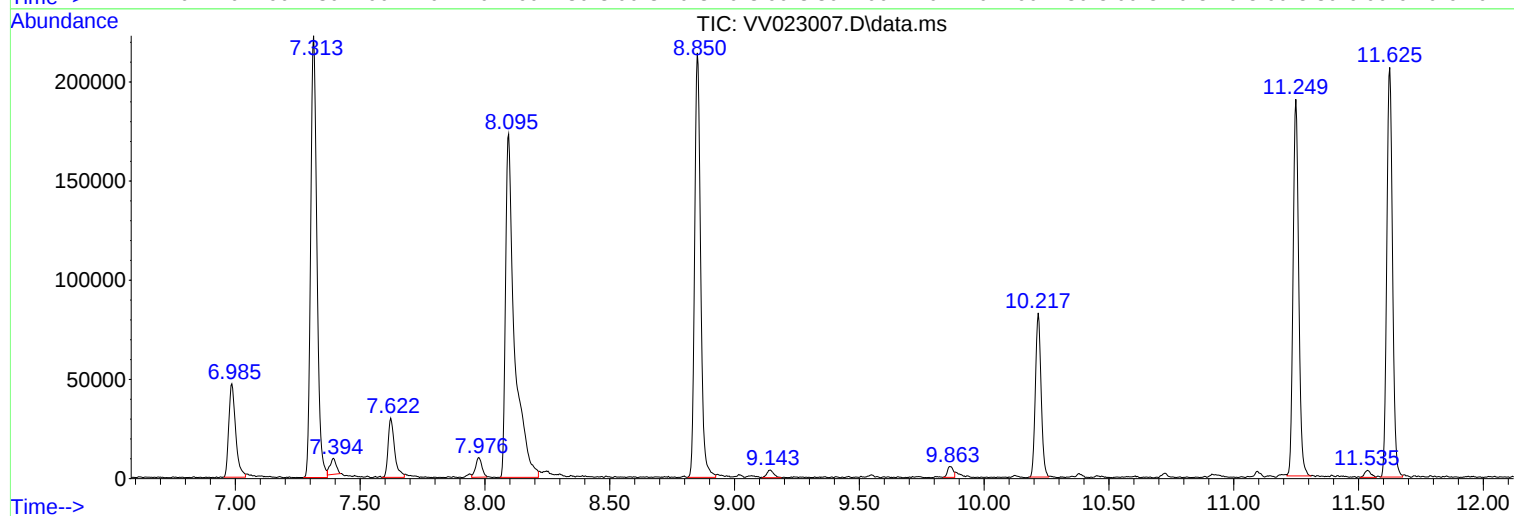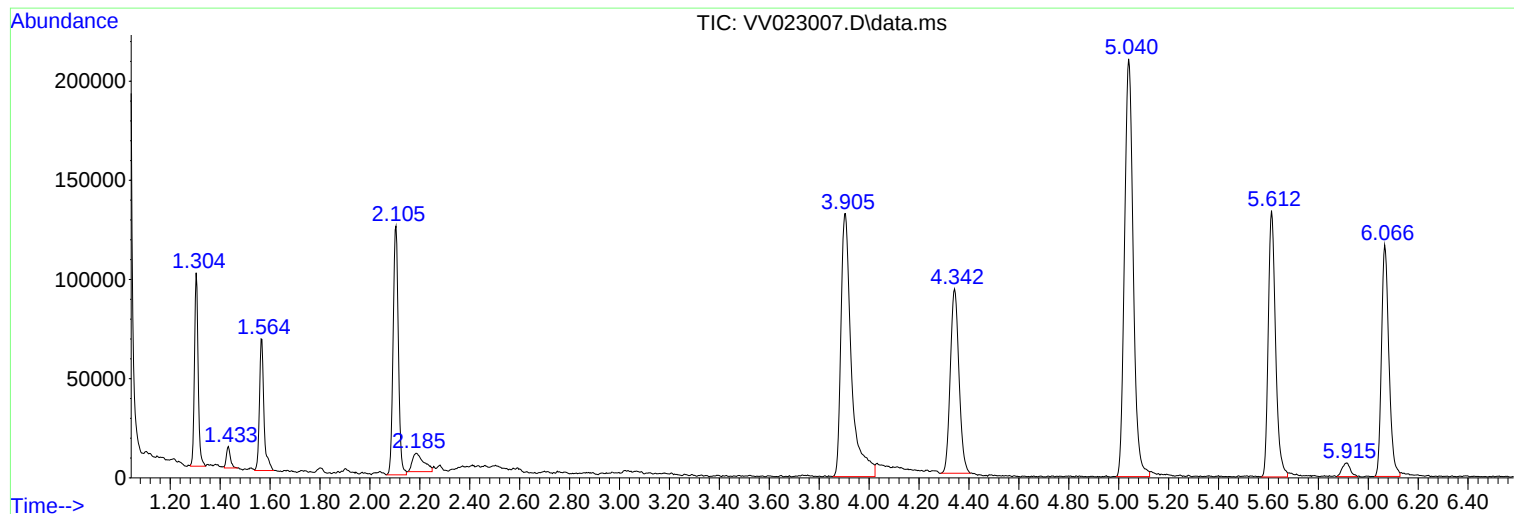

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023007.D
Acq On : 23 Oct 2021 14:11
Operator : SY/MD
Sample : M4277-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023007.D
Acq On : 23 Oct 2021 14:11
Operator : SY/MD
Sample : M4277-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc