

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023008.D
 Acq On : 23 Oct 2021 14:35
 Operator : SY/MD
 Sample : M4277-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGA1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023008.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	97	rVB	86099	89462	18.52%	2.221%
2	1.568	156	164	175	rBV	57455	64754	13.41%	1.607%
3	2.108	318	332	352	rBV	126754	186613	38.64%	4.632%
4	2.770	523	538	553	rBV3	9240	21444	4.44%	0.532%
5	3.899	878	889	937	rBV2	42385	179939	37.25%	4.466%
6	4.349	1012	1029	1057	rBV	85806	219034	45.35%	5.437%
7	5.047	1230	1246	1268	rBV3	192103	483014	100.00%	11.989%
8	5.619	1411	1424	1442	rBV	135292	275026	56.94%	6.827%
9	6.072	1551	1565	1592	rBV2	112688	236080	48.88%	5.860%
10	6.989	1839	1850	1865	rBV2	45863	86868	17.98%	2.156%
11	7.317	1940	1952	1965	rBV	215782	375092	77.66%	9.310%
12	7.391	1965	1975	1999	rVB	121528	219431	45.43%	5.447%
13	7.625	2039	2048	2069	rBV	29323	52930	10.96%	1.314%
14	7.979	2152	2158	2169	rVB7	4025	6524	1.35%	0.162%
15	8.091	2182	2193	2227	rBV	208045	430795	89.19%	10.693%
16	8.853	2419	2430	2450	rBV	217708	360152	74.56%	8.940%
17	9.146	2509	2521	2531	rBV4	3860	6981	1.45%	0.173%
18	10.217	2844	2854	2869	rBV	79533	128707	26.65%	3.195%
19	11.249	3166	3175	3197	rVB	186429	293797	60.83%	7.293%
20	11.625	3280	3292	3311	rBV	194778	312060	64.61%	7.746%




Sum of corrected areas: 4028703

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023008.D
Acq On : 23 Oct 2021 14:35
Operator : SY/MD
Sample : M4277-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

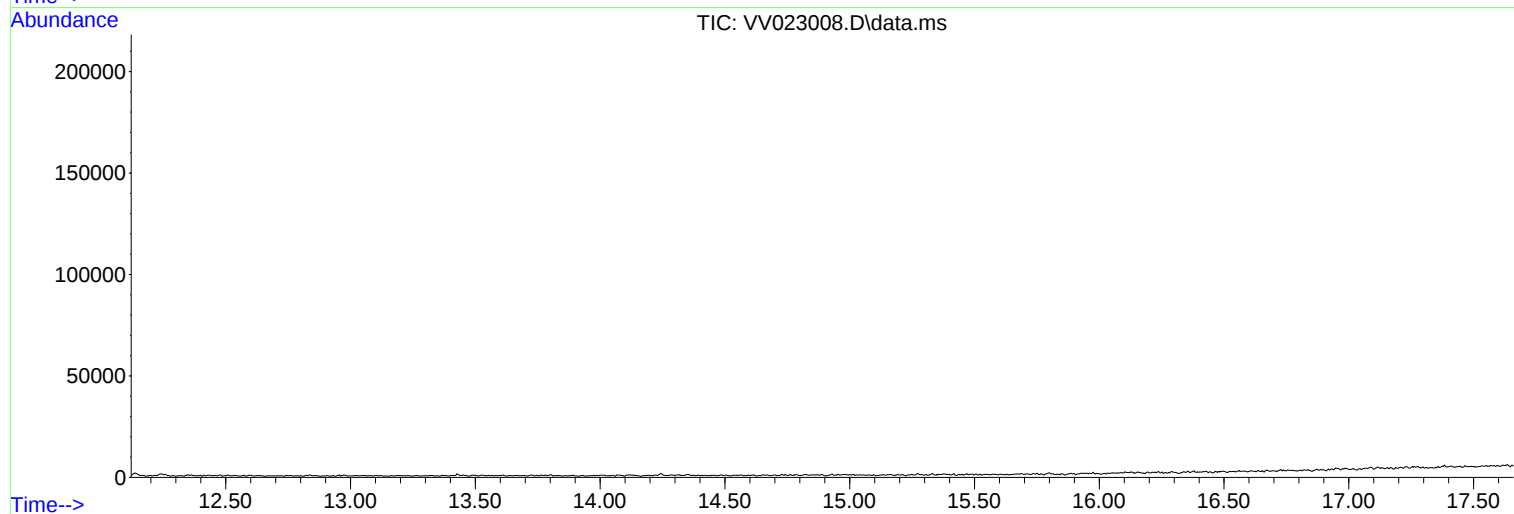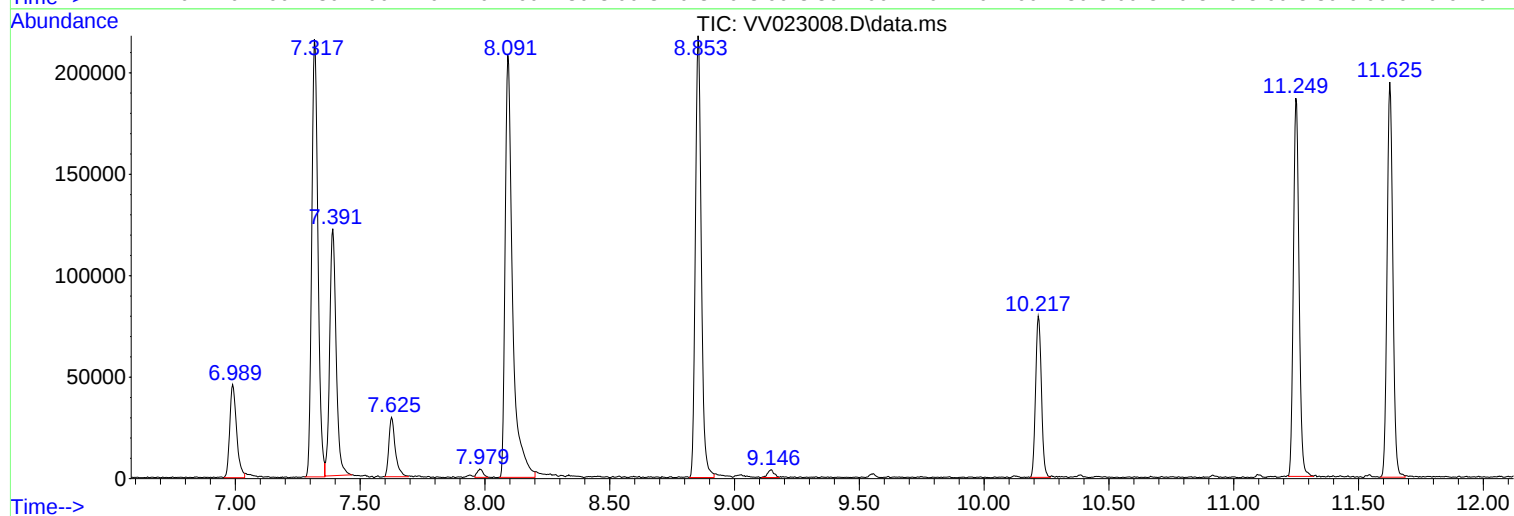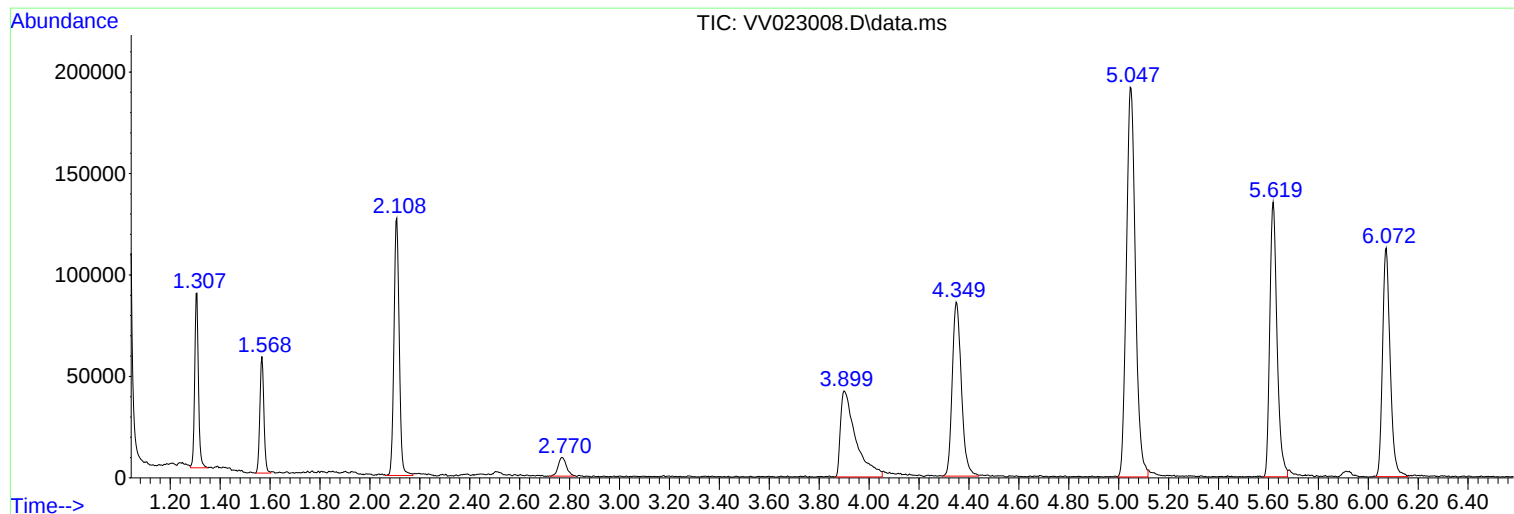

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023008.D
Acq On : 23 Oct 2021 14:35
Operator : SY/MD
Sample : M4277-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023008.D
Acq On : 23 Oct 2021 14:35
Operator : SY/MD
Sample : M4277-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
