

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023009.D
 Acq On : 23 Oct 2021 14:59
 Operator : SY/MD
 Sample : M4277-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGA5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023009.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rVB	93266	102190	6.85%	1.812%
2	1.568	155	164	178	rBV	61717	71325	4.78%	1.265%
3	2.108	321	332	346	rBV	113503	163196	10.94%	2.894%
4	3.902	877	890	930	rBV	52164	209405	14.04%	3.713%
5	4.352	1014	1030	1057	rBV2	91887	243579	16.33%	4.319%
6	5.047	1229	1246	1273	rBV2	204034	518433	34.75%	9.193%
7	5.619	1412	1424	1449	rBV	135396	277684	18.61%	4.924%
8	5.918	1504	1517	1539	rBV	69950	147149	9.86%	2.609%
9	6.072	1549	1565	1586	rBV2	120682	249871	16.75%	4.431%
10	6.989	1837	1850	1869	rBV	50303	94738	6.35%	1.680%
11	7.320	1939	1953	1970	rBV	229756	409194	27.43%	7.256%
12	7.397	1970	1977	1990	rVB3	7840	16632	1.11%	0.295%
13	7.625	2039	2048	2065	rBV2	31338	56051	3.76%	0.994%
14	7.976	2137	2157	2179	rBV	894047	1491846	100.00%	26.455%
15	8.092	2183	2193	2224	rVV	231693	453522	30.40%	8.042%
16	8.854	2418	2430	2448	rBV	220110	359051	24.07%	6.367%
17	10.217	2841	2854	2869	rBV	85197	136040	9.12%	2.412%
18	11.249	3165	3175	3195	rVB	190837	299378	20.07%	5.309%
19	11.625	3281	3292	3311	rBV	214469	339987	22.79%	6.029%




Sum of corrected areas: 5639271

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023009.D
Acq On : 23 Oct 2021 14:59
Operator : SY/MD
Sample : M4277-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

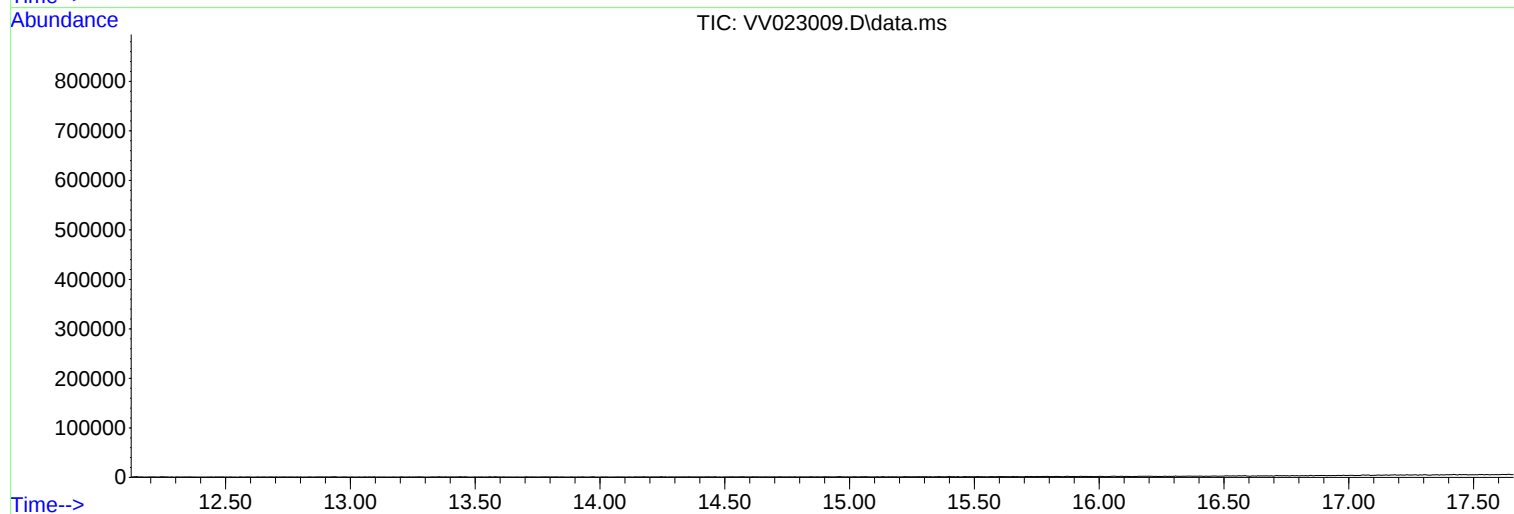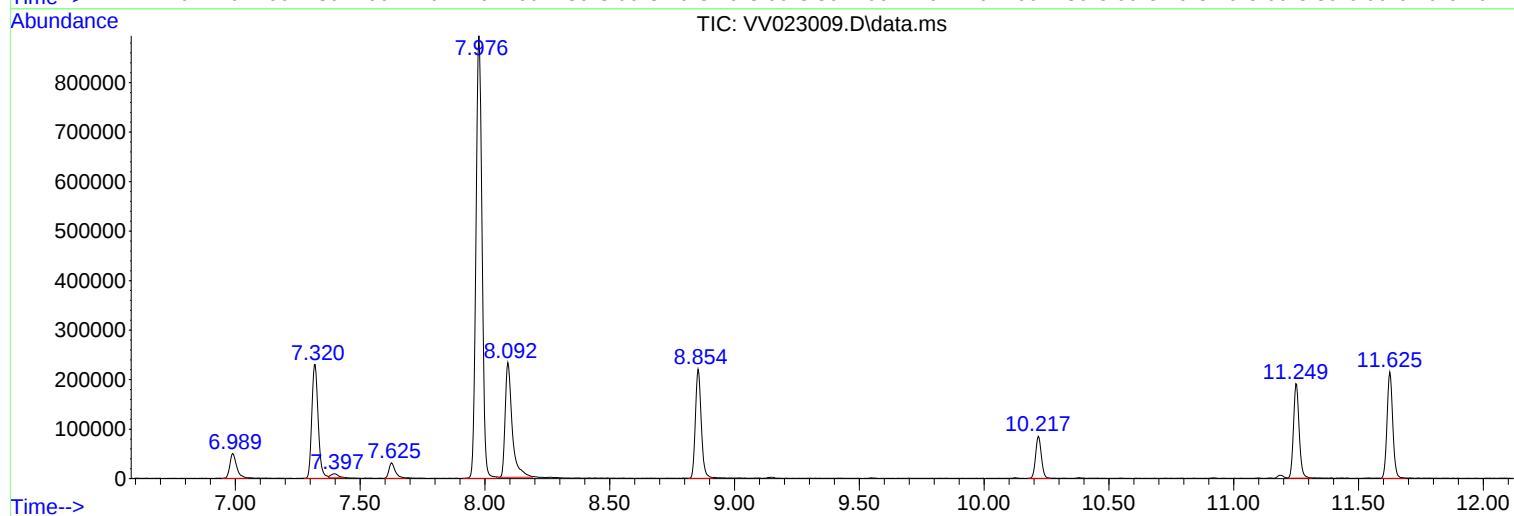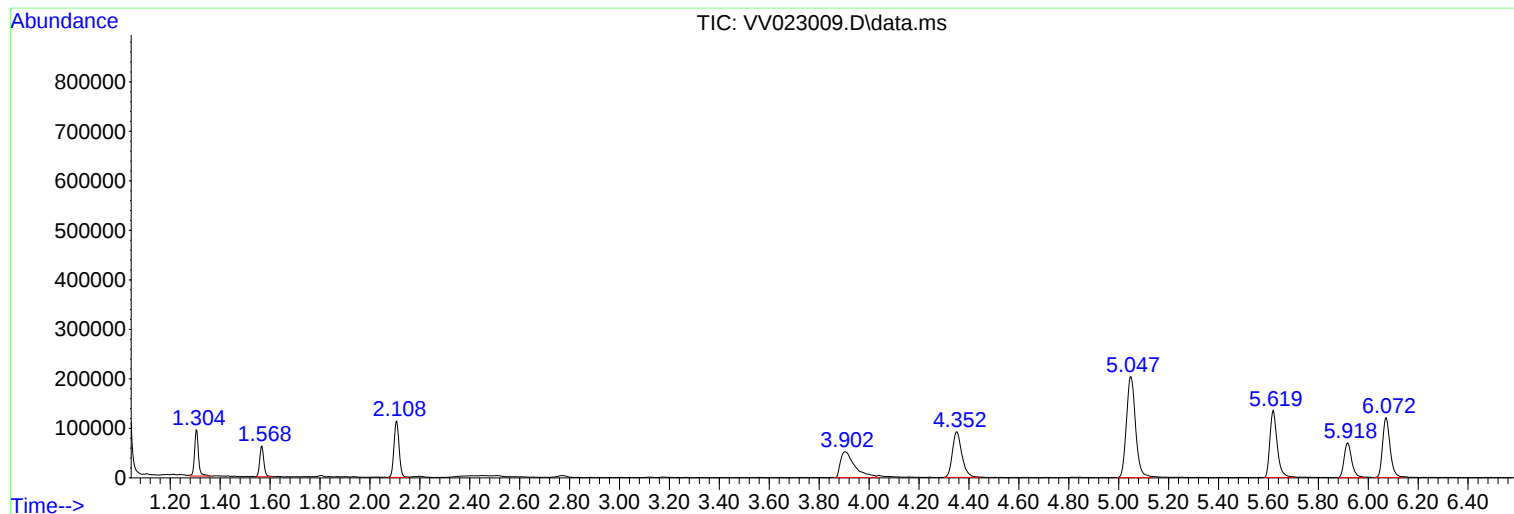

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023009.D
Acq On : 23 Oct 2021 14:59
Operator : SY/MD
Sample : M4277-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023009.D
Acq On : 23 Oct 2021 14:59
Operator : SY/MD
Sample : M4277-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc