

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023010.D
 Acq On : 23 Oct 2021 15:23
 Operator : SY/MD
 Sample : M4277-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGA7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023010.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rVB	95500	103736	10.60%	1.788%
2	1.568	154	164	176	rBV	59512	68344	6.98%	1.178%
3	2.108	321	332	348	rBV	119316	172563	17.63%	2.974%
4	2.767	527	537	549	rBV3	9636	19762	2.02%	0.341%
5	3.908	874	892	928	rBV2	279373	794784	81.20%	13.698%
6	4.349	1011	1029	1053	rBV2	93928	240805	24.60%	4.150%
7	5.050	1227	1247	1274	rBV2	207218	527720	53.92%	9.095%
8	5.619	1411	1424	1442	rBV	139625	284175	29.03%	4.898%
9	5.918	1504	1517	1535	rBV	74255	154701	15.81%	2.666%
10	6.072	1552	1565	1592	rBV	117738	250882	25.63%	4.324%
11	6.989	1839	1850	1868	rBV	49879	94478	9.65%	1.628%
12	7.317	1939	1952	1969	rBV	232452	409929	41.88%	7.065%
13	7.394	1971	1976	1990	rVB	8444	16074	1.64%	0.277%
14	7.625	2036	2048	2068	rBV	31284	57609	5.89%	0.993%
15	7.976	2143	2157	2177	rBV	583733	978790	100.00%	16.870%
16	8.092	2183	2193	2224	rBV	240349	458604	46.85%	7.904%
17	8.854	2416	2430	2455	rBV	224370	370672	37.87%	6.389%
18	10.217	2843	2854	2868	rBV	87813	136020	13.90%	2.344%
19	11.249	3165	3175	3194	rVV	200282	311641	31.84%	5.371%
20	11.625	3280	3292	3312	rBV	220014	350812	35.84%	6.046%




Sum of corrected areas: 5802101

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023010.D
Acq On : 23 Oct 2021 15:23
Operator : SY/MD
Sample : M4277-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

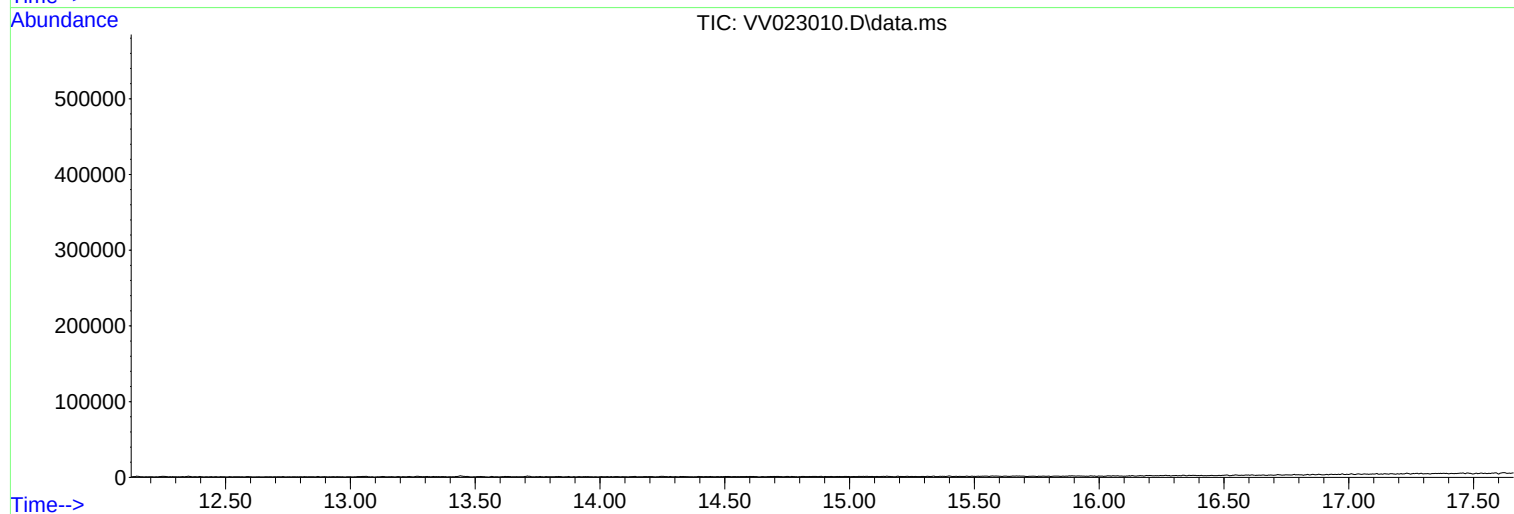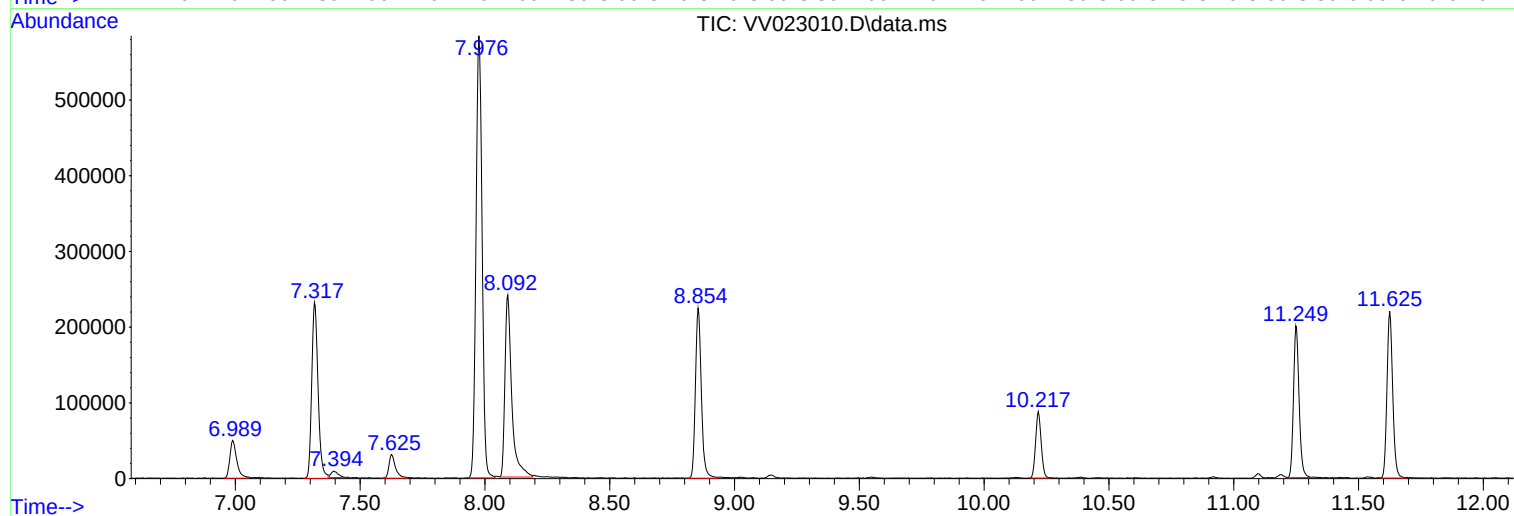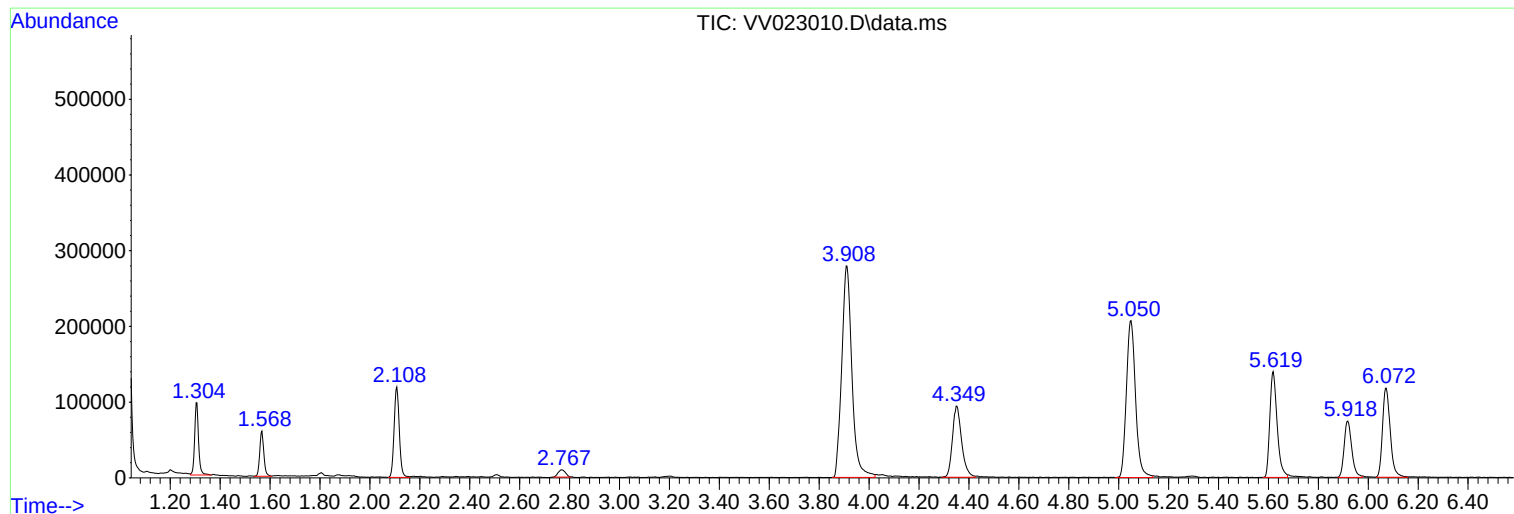

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023010.D
Acq On : 23 Oct 2021 15:23
Operator : SY/MD
Sample : M4277-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023010.D
Acq On : 23 Oct 2021 15:23
Operator : SY/MD
Sample : M4277-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc