

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023013.D
 Acq On : 23 Oct 2021 16:35
 Operator : SY/MD
 Sample : M4277-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGB3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023013.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	90609	93747	17.87%	2.221%
2	1.568	155	164	175	rBV	59336	70032	13.35%	1.659%
3	2.105	320	331	345	rBV	125516	182065	34.70%	4.314%
4	2.195	347	359	373	rVB2	5381	16416	3.13%	0.389%
5	3.905	877	891	926	rBV2	59832	227601	43.38%	5.393%
6	4.349	1012	1029	1056	rBV	90879	230734	43.98%	5.468%
7	5.047	1230	1246	1275	rBV2	207059	524626	100.00%	12.432%
8	5.619	1411	1424	1451	rBV	133458	278380	53.06%	6.597%
9	5.921	1506	1518	1534	rBV10	8039	18548	3.54%	0.440%
10	6.072	1550	1565	1588	rBV	119737	249456	47.55%	5.911%
11	6.989	1838	1850	1866	rBV2	49733	93806	17.88%	2.223%
12	7.317	1939	1952	1966	rBV	230851	409928	78.14%	9.714%
13	7.391	1967	1975	1995	rVB	66221	121262	23.11%	2.873%
14	7.625	2035	2048	2065	rBV	30192	54830	10.45%	1.299%
15	7.979	2147	2158	2176	rVB	45084	78320	14.93%	1.856%
16	8.092	2183	2193	2224	rBV	229165	454845	86.70%	10.778%
17	8.854	2418	2430	2452	rBV	212845	352754	67.24%	8.359%
18	10.217	2838	2854	2872	rBV	85050	134294	25.60%	3.182%
19	11.249	3165	3175	3189	rBV	183328	289666	55.21%	6.864%
20	11.625	3281	3292	3318	rBV2	210593	338787	64.58%	8.028%




Sum of corrected areas: 4220097

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023013.D
Acq On : 23 Oct 2021 16:35
Operator : SY/MD
Sample : M4277-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

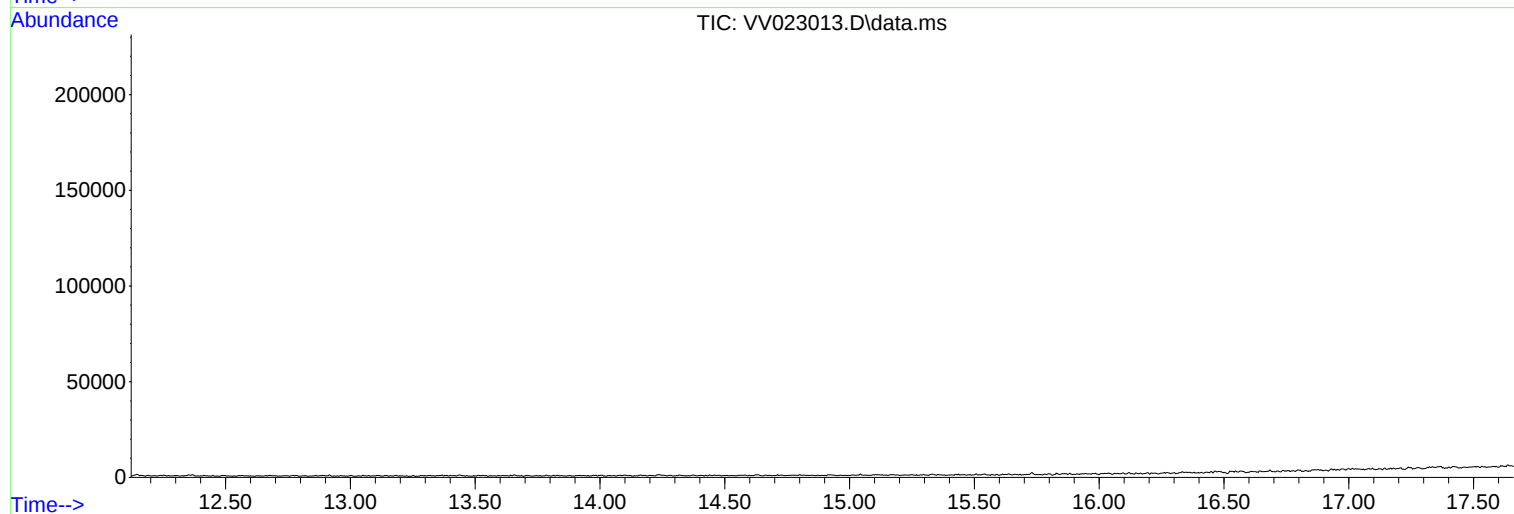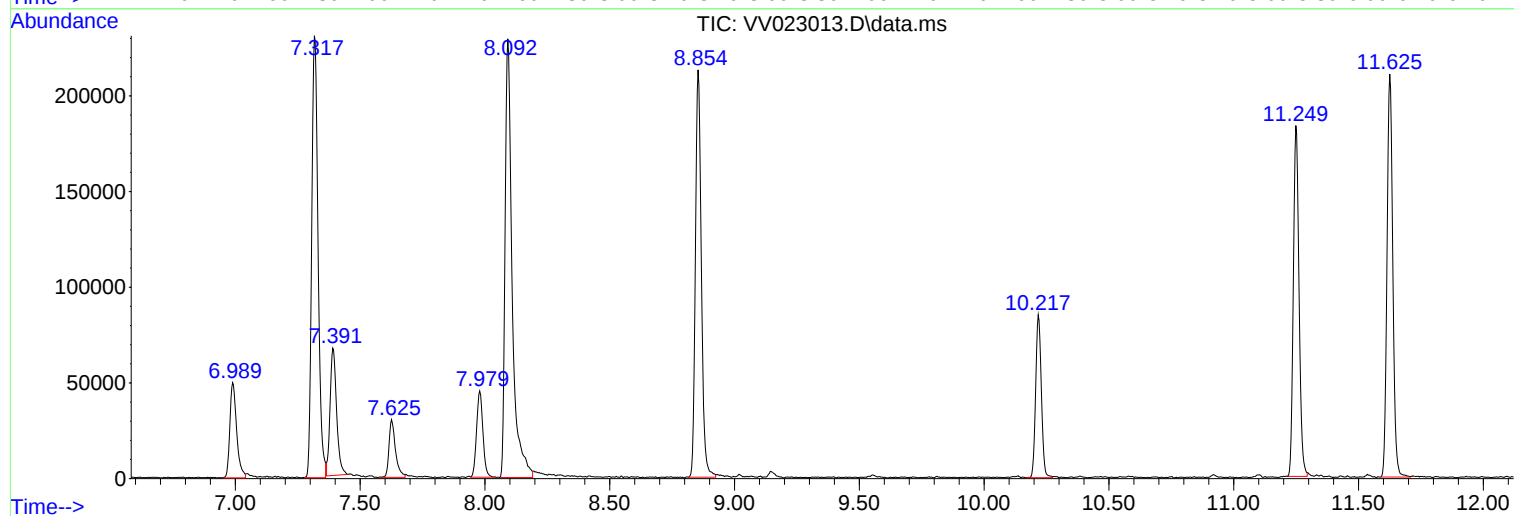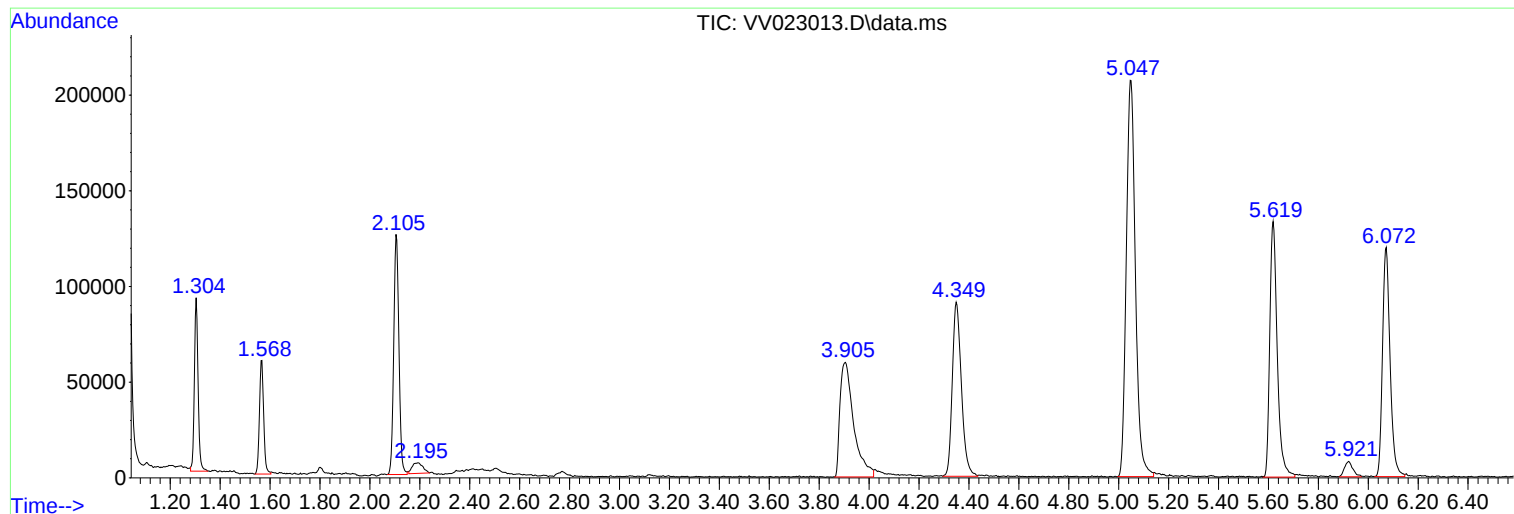

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023013.D
Acq On : 23 Oct 2021 16:35
Operator : SY/MD
Sample : M4277-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023013.D
Acq On : 23 Oct 2021 16:35
Operator : SY/MD
Sample : M4277-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
