

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023014.D
 Acq On : 23 Oct 2021 16:59
 Operator : SY/MD
 Sample : M4277-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGB4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	95	rVB	92696	98789	9.48%	1.873%
2	1.568	156	164	179	rVB	60180	69431	6.66%	1.317%
3	2.105	320	331	346	rBV	103707	150786	14.47%	2.859%
4	2.767	524	537	551	rBV5	17079	37978	3.64%	0.720%
5	3.908	877	892	922	rBV2	401098	1042307	100.00%	19.765%
6	4.349	1012	1029	1054	rBV	90497	230096	22.08%	4.363%
7	5.047	1230	1246	1271	rBV3	211765	523050	50.18%	9.918%
8	5.619	1411	1424	1448	rBV	143375	296710	28.47%	5.626%
9	5.918	1505	1517	1536	rBV2	64399	132767	12.74%	2.518%
10	6.072	1549	1565	1584	rBV2	116853	245405	23.54%	4.653%
11	6.989	1839	1850	1870	rBV	47942	92375	8.86%	1.752%
12	7.317	1941	1952	1968	rBV	231809	411615	39.49%	7.805%
13	7.394	1968	1976	1991	rVB	28118	51987	4.99%	0.986%
14	7.625	2039	2048	2067	rBV	28922	53888	5.17%	1.022%
15	7.976	2142	2157	2174	rBV3	112390	194662	18.68%	3.691%
16	8.095	2183	2194	2228	rBV	196614	463123	44.43%	8.782%
17	8.854	2419	2430	2451	rBV	222399	373322	35.82%	7.079%
18	10.220	2844	2855	2871	rBV	85495	139249	13.36%	2.641%
19	11.249	3165	3175	3196	rBV	198286	316166	30.33%	5.995%
20	11.625	3278	3292	3308	rBV	221698	349875	33.57%	6.634%




Sum of corrected areas: 5273581

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023014.D
Acq On : 23 Oct 2021 16:59
Operator : SY/MD
Sample : M4277-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

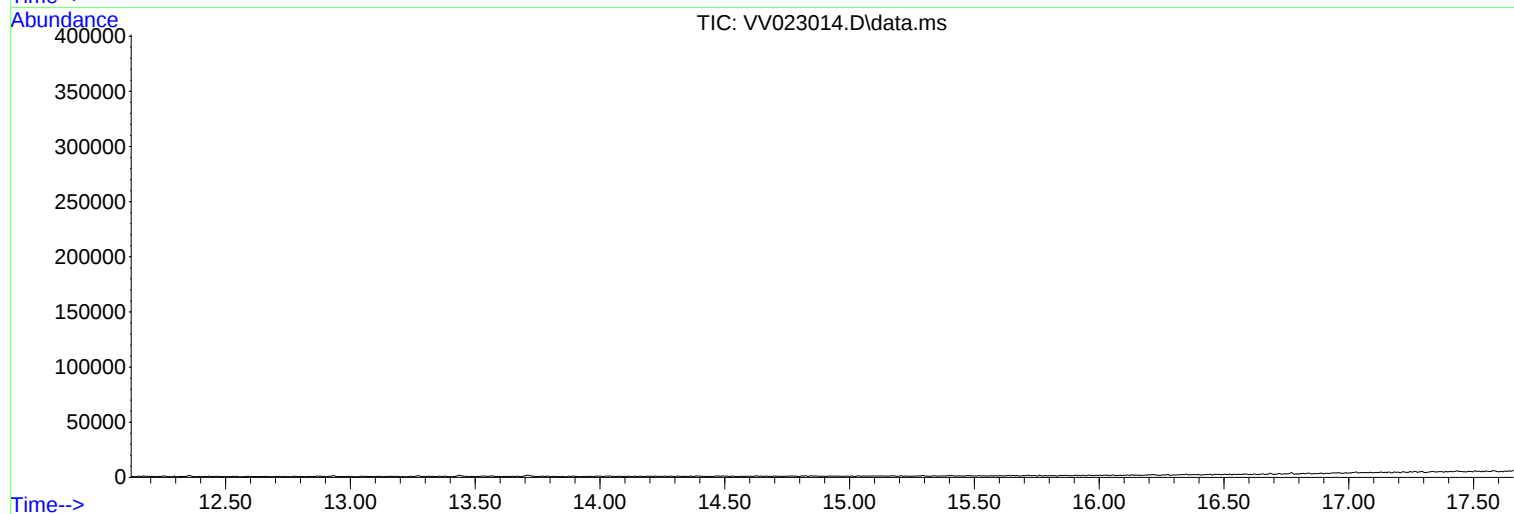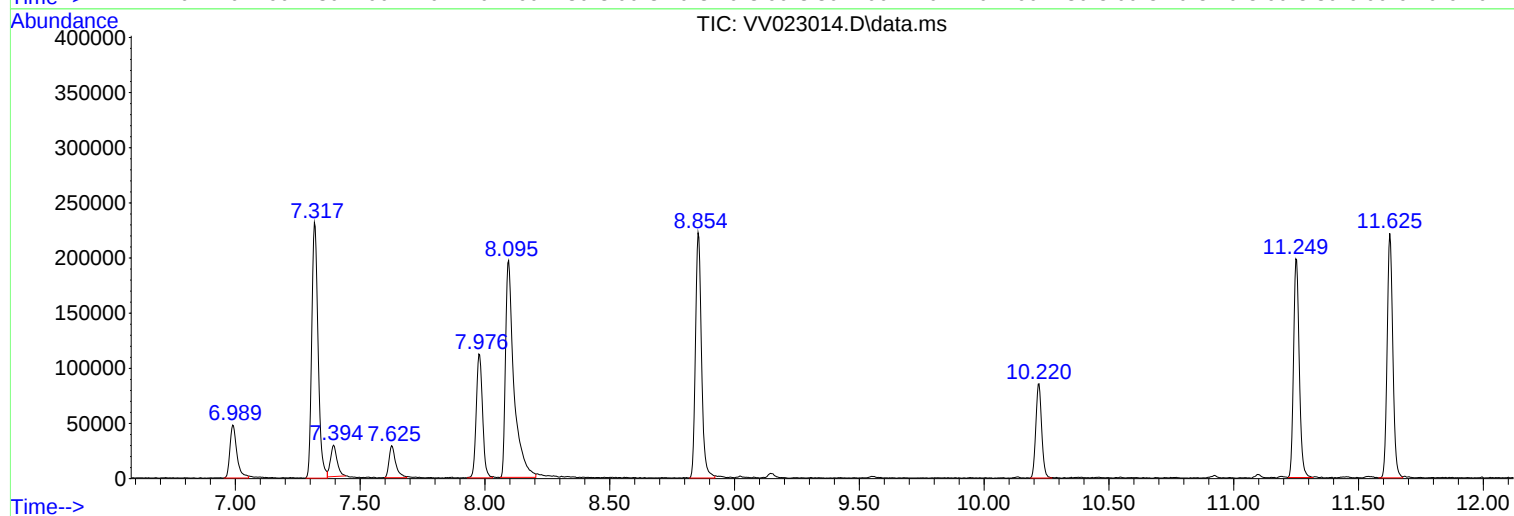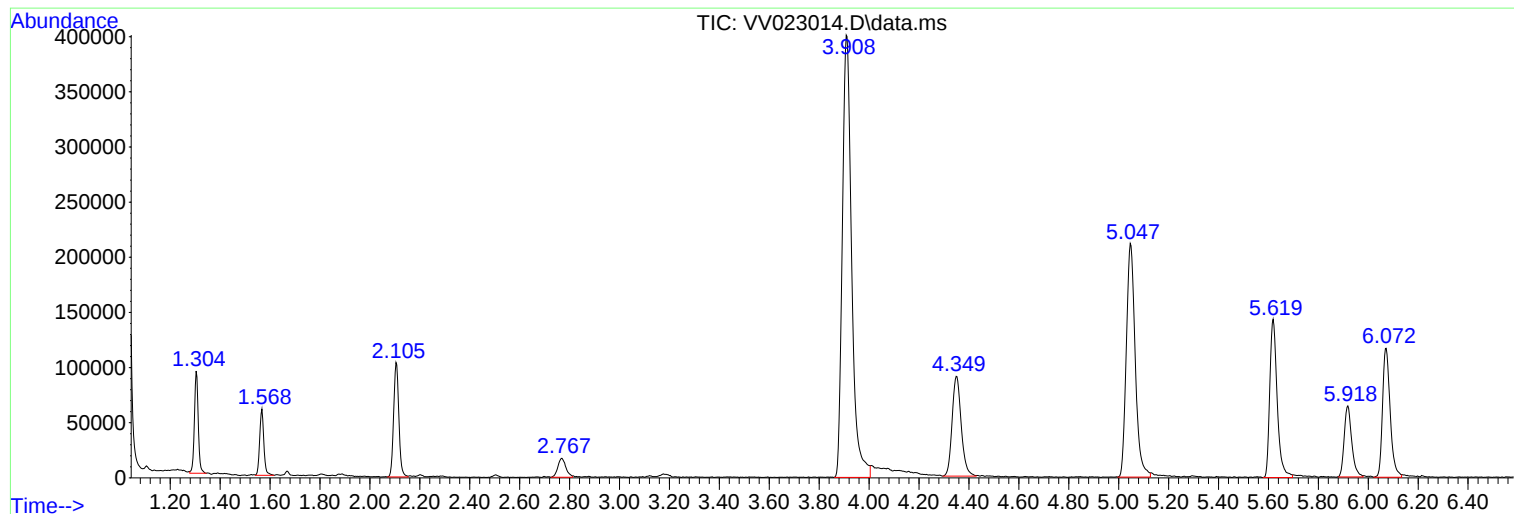

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023014.D
Acq On : 23 Oct 2021 16:59
Operator : SY/MD
Sample : M4277-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023014.D
Acq On : 23 Oct 2021 16:59
Operator : SY/MD
Sample : M4277-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc