

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023015.D
 Acq On : 23 Oct 2021 17:23
 Operator : SY/MD
 Sample : M4277-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFG6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	94	rVB	70404	72360	16.87%	2.156%
2	1.564	155	163	171	rBV	42594	48475	11.30%	1.444%
3	2.105	321	331	344	rBV	80286	115633	26.95%	3.445%
4	2.172	344	352	360	rVB	3926	6413	1.49%	0.191%
5	3.883	874	884	918	rBV2	58612	180808	42.14%	5.387%
6	4.349	1014	1029	1056	rBV	70496	183117	42.68%	5.456%
7	5.050	1230	1247	1271	rBV3	161427	411000	95.80%	12.245%
8	5.619	1413	1424	1446	rBV	104016	216301	50.42%	6.445%
9	5.918	1503	1517	1535	rVB	6591	16311	3.80%	0.486%
10	6.072	1552	1565	1586	rBV	93954	197561	46.05%	5.886%
11	6.178	1588	1598	1613	rVB4	12085	26017	6.06%	0.775%
12	6.989	1840	1850	1870	rBV	39806	76465	17.82%	2.278%
13	7.317	1938	1952	1967	rBV	174035	307703	71.72%	9.168%
14	7.394	1967	1976	1995	rVB	37178	72524	16.90%	2.161%
15	7.625	2035	2048	2064	rBV2	25859	47222	11.01%	1.407%
16	7.979	2144	2158	2170	rBV3	41028	69671	16.24%	2.076%
17	8.092	2180	2193	2224	rBV2	218452	429029	100.00%	12.783%
18	8.854	2415	2430	2448	rBV	164956	275703	64.26%	8.214%
19	10.217	2843	2854	2869	rBV	78061	123583	28.81%	3.682%
20	11.249	3165	3175	3192	rBV	140672	221235	51.57%	6.592%
21	11.625	3281	3292	3308	rBV	161851	259205	60.42%	7.723%




Sum of corrected areas: 3356336

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023015.D
Acq On : 23 Oct 2021 17:23
Operator : SY/MD
Sample : M4277-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

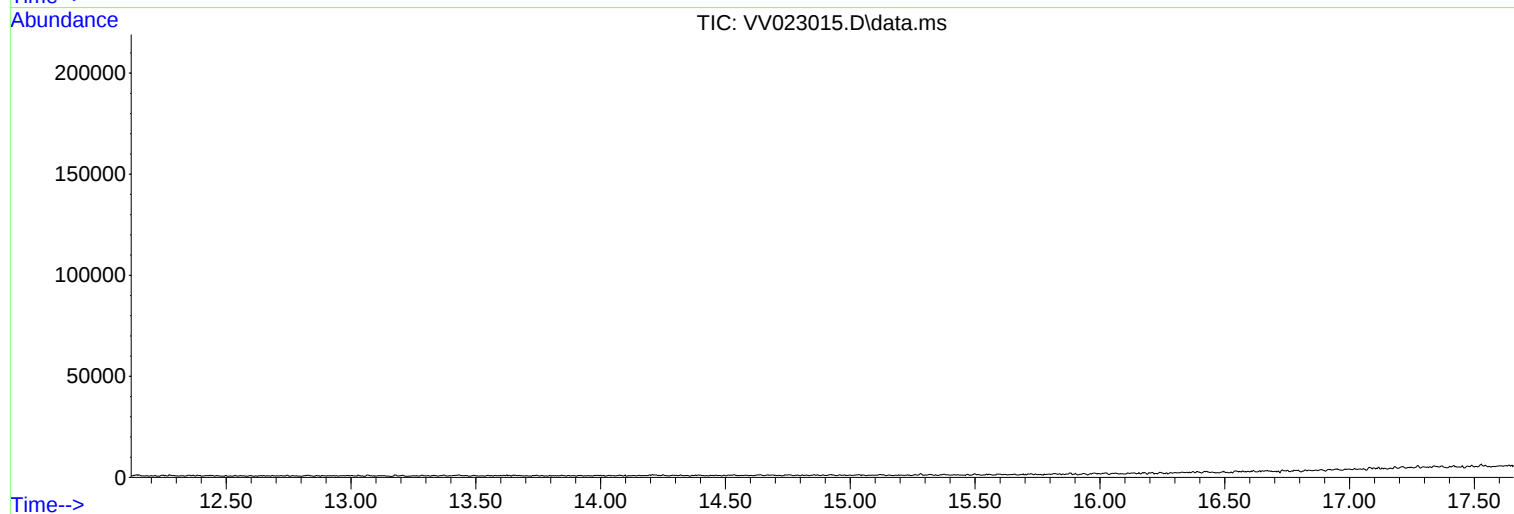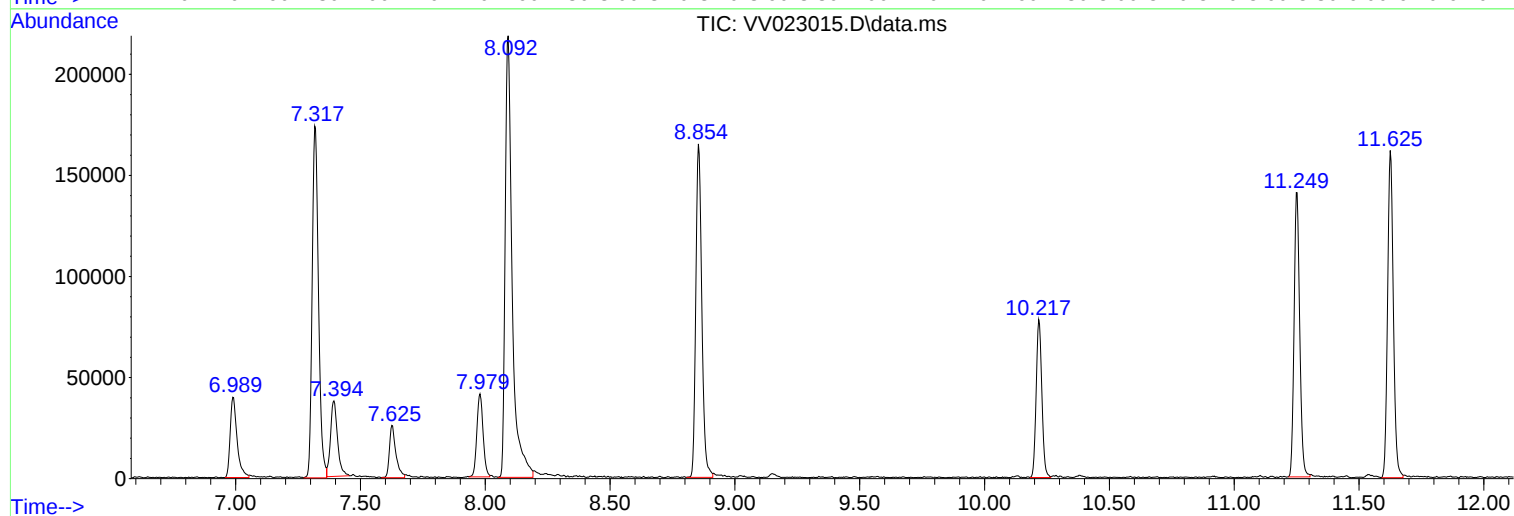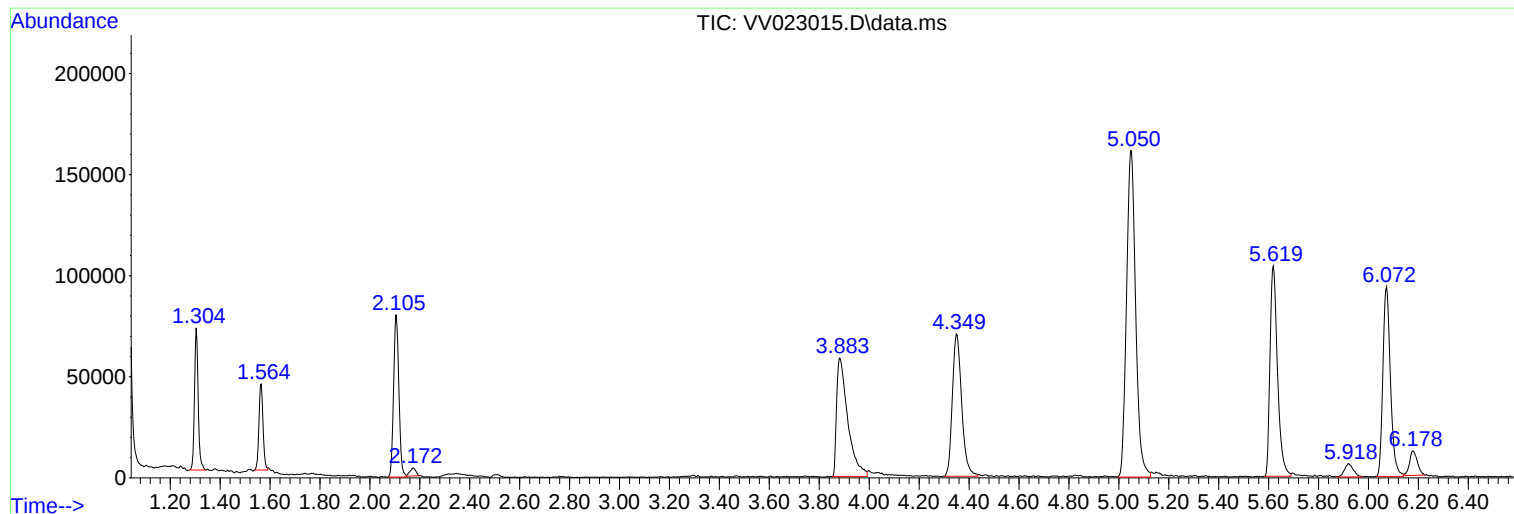

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023015.D
Acq On : 23 Oct 2021 17:23
Operator : SY/MD
Sample : M4277-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023015.D
Acq On : 23 Oct 2021 17:23
Operator : SY/MD
Sample : M4277-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc