

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023018.D
 Acq On : 23 Oct 2021 18:35
 Operator : SY/MD
 Sample : M4277-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGB9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	70194	72123	16.09%	2.213%
2	1.568	156	164	172	rBV	46084	52952	11.81%	1.625%
3	2.105	321	331	345	rBV	78745	112865	25.18%	3.463%
4	3.902	877	890	935	rBV2	47493	192548	42.96%	5.907%
5	4.352	1013	1030	1056	rBV4	73672	215698	48.12%	6.618%
6	5.050	1230	1247	1271	rBV2	163025	412238	91.97%	12.647%
7	5.619	1412	1424	1448	rBV	103359	215230	48.02%	6.603%
8	5.918	1505	1517	1528	rBV	3606	8934	1.99%	0.274%
9	6.072	1551	1565	1587	rBV2	95191	201205	44.89%	6.173%
10	6.989	1838	1850	1864	rBV	38934	73512	16.40%	2.255%
11	7.317	1940	1952	1969	rBV	170227	302689	67.53%	9.286%
12	7.400	1970	1978	1988	rVB2	7467	13825	3.08%	0.424%
13	7.625	2039	2048	2067	rBV2	24209	44841	10.00%	1.376%
14	7.979	2150	2158	2170	rVB3	8747	13905	3.10%	0.427%
15	8.092	2182	2193	2235	rBV2	218389	448246	100.00%	13.752%
16	8.854	2419	2430	2458	rBV	163905	274316	61.20%	8.416%
17	10.217	2841	2854	2871	rBV	78237	123306	27.51%	3.783%
18	11.249	3165	3175	3191	rBV	139362	217789	48.59%	6.682%
19	11.535	3257	3264	3273	rBV5	2825	4730	1.06%	0.145%
20	11.625	3281	3292	3309	rBV	162656	258533	57.68%	7.932%




Sum of corrected areas: 3259485

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023018.D
Acq On : 23 Oct 2021 18:35
Operator : SY/MD
Sample : M4277-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

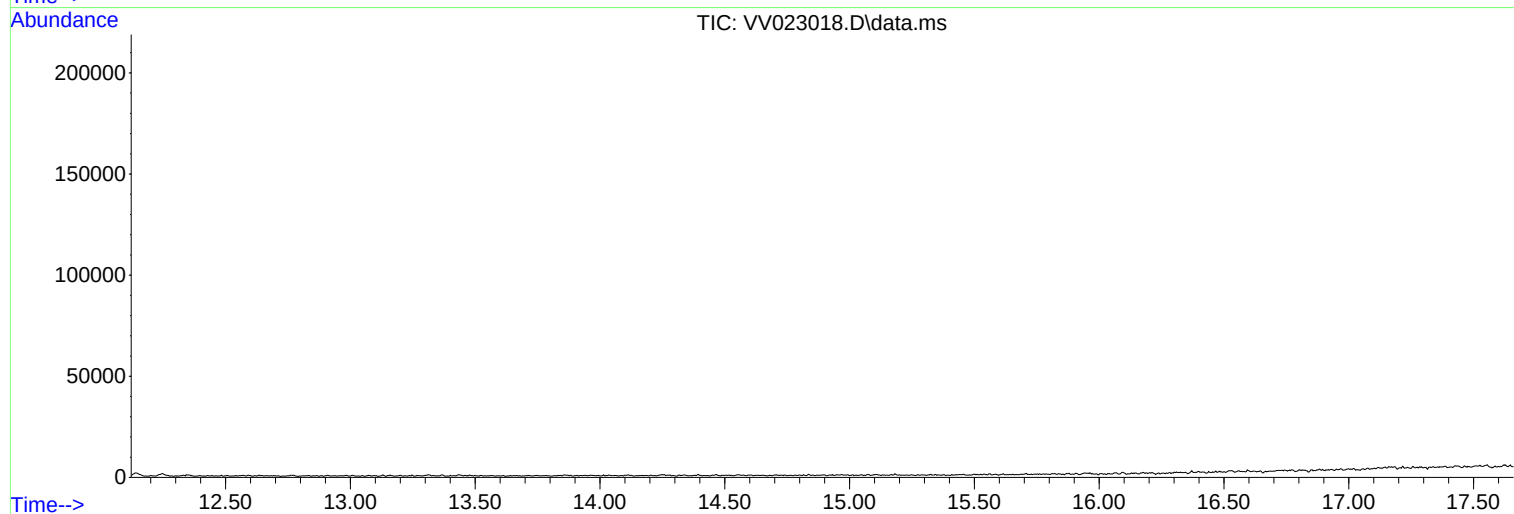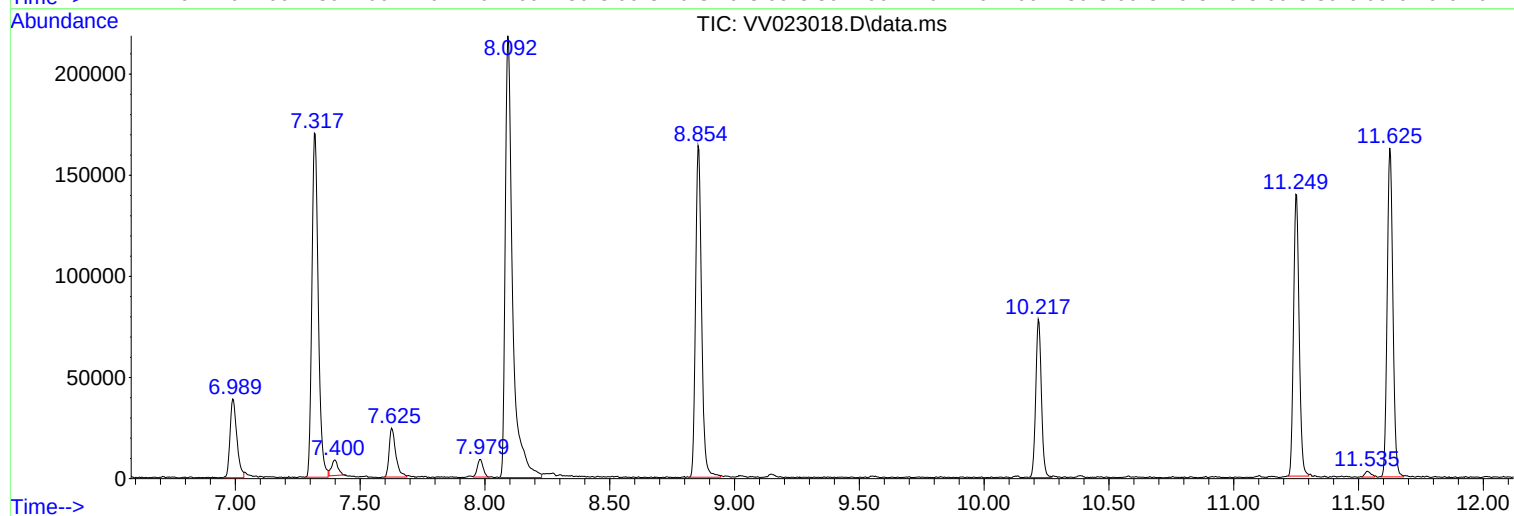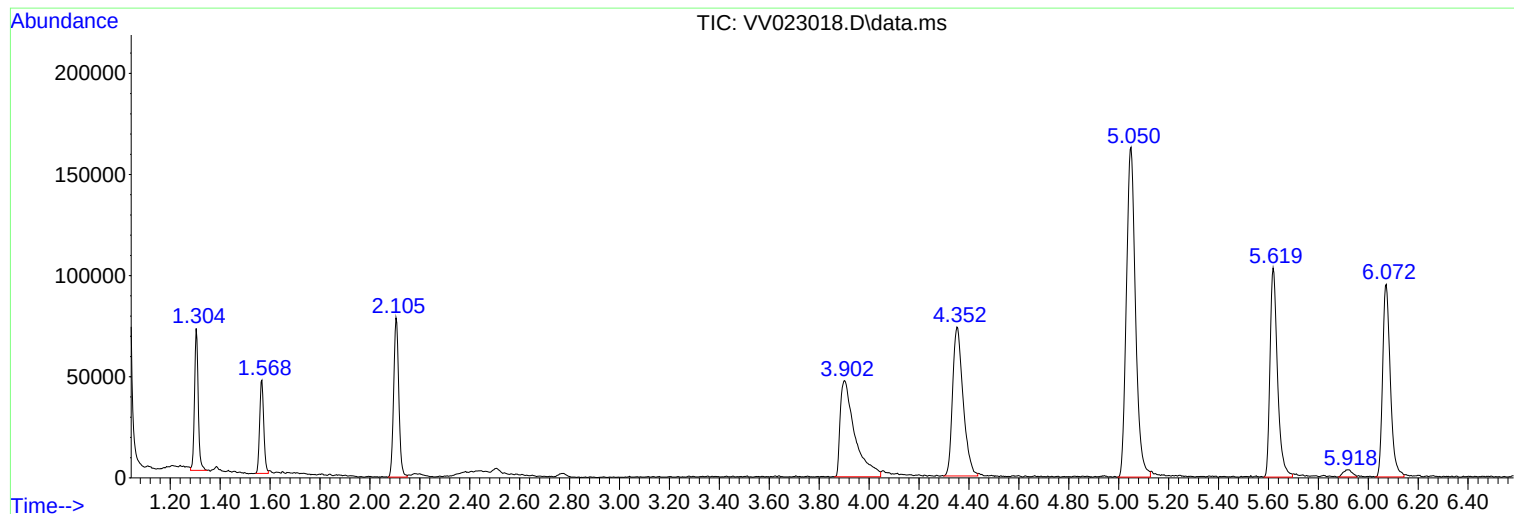

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023018.D
Acq On : 23 Oct 2021 18:35
Operator : SY/MD
Sample : M4277-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023018.D
Acq On : 23 Oct 2021 18:35
Operator : SY/MD
Sample : M4277-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc