

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023019.D
 Acq On : 23 Oct 2021 18:59
 Operator : SY/MD
 Sample : M4277-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGD8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	73096	78030	4.42%	1.260%
2	1.564	155	163	175	rBV	54367	63679	3.61%	1.028%
3	2.108	322	332	342	rBV	99384	144417	8.18%	2.332%
4	2.175	342	353	380	rVB	73367	172071	9.74%	2.779%
5	2.349	383	407	410	rBV	24886	73886	4.18%	1.193%
6	3.908	870	892	920	rBV2	694151	1765762	100.00%	28.517%
7	4.349	1014	1029	1056	rBV2	85062	215247	12.19%	3.476%
8	5.050	1226	1247	1271	rBV3	188517	475331	26.92%	7.677%
9	5.619	1413	1424	1453	rBV	125576	260364	14.75%	4.205%
10	5.918	1500	1517	1535	rBV	84093	175321	9.93%	2.831%
11	6.072	1550	1565	1585	rBV	110587	231268	13.10%	3.735%
12	6.989	1840	1850	1874	rBV2	45101	86752	4.91%	1.401%
13	7.317	1937	1952	1970	rBV	194151	342680	19.41%	5.534%
14	7.625	2037	2048	2063	rBV2	26109	48015	2.72%	0.775%
15	7.976	2144	2157	2182	rBV	360600	606590	34.35%	9.796%
16	8.091	2182	2193	2234	rVV	217807	425672	24.11%	6.875%
17	8.854	2419	2430	2454	rBV	193680	327379	18.54%	5.287%
18	10.217	2843	2854	2867	rBV	79336	126963	7.19%	2.050%
19	11.249	3165	3175	3198	rVV	166218	271489	15.38%	4.385%
20	11.625	3280	3292	3314	rVB	183289	301096	17.05%	4.863%




Sum of corrected areas: 6192012

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023019.D
Acq On : 23 Oct 2021 18:59
Operator : SY/MD
Sample : M4277-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

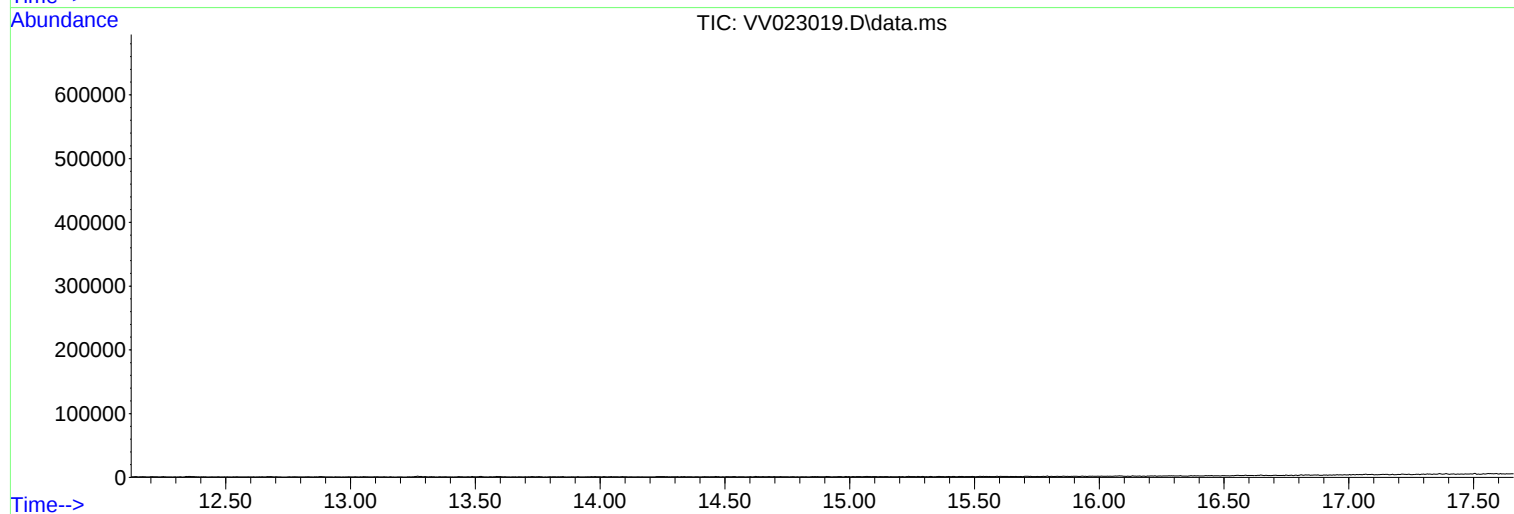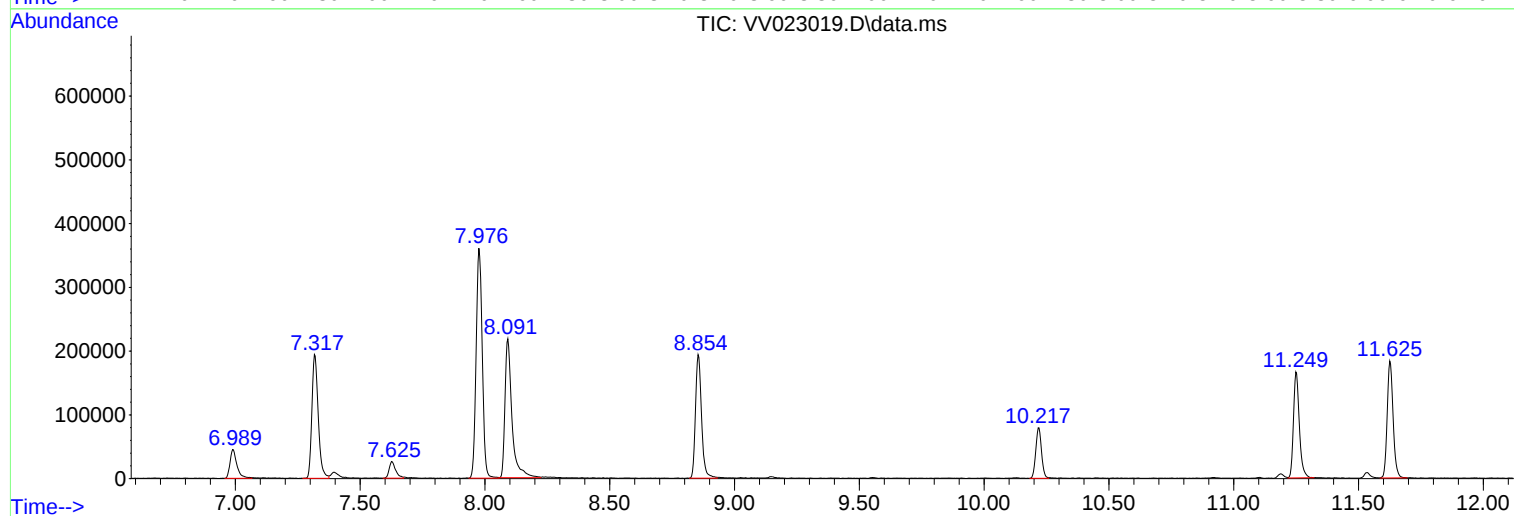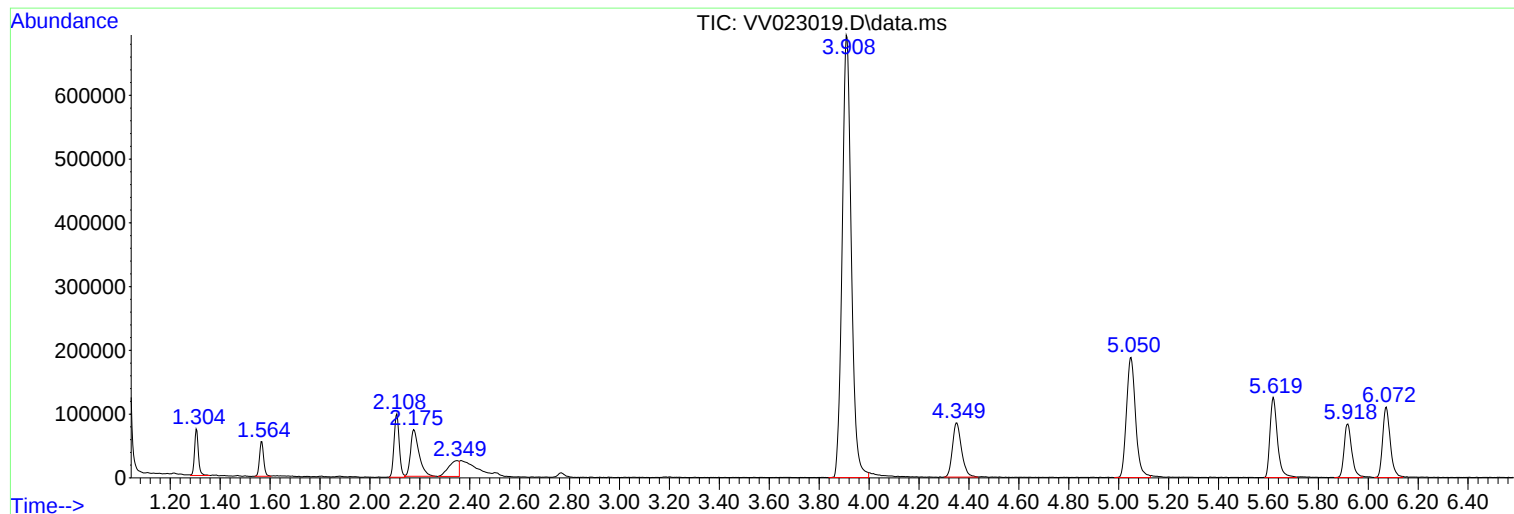

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023019.D
Acq On : 23 Oct 2021 18:59
Operator : SY/MD
Sample : M4277-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.349	1.42 ug/L	73886	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	56
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	56

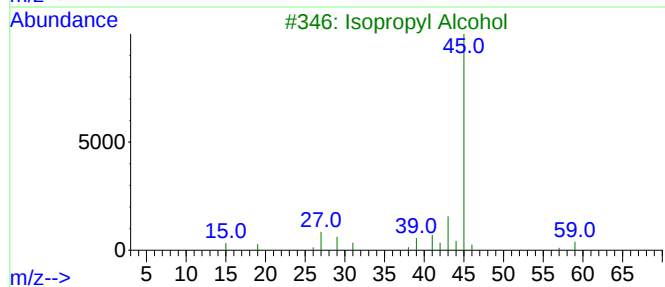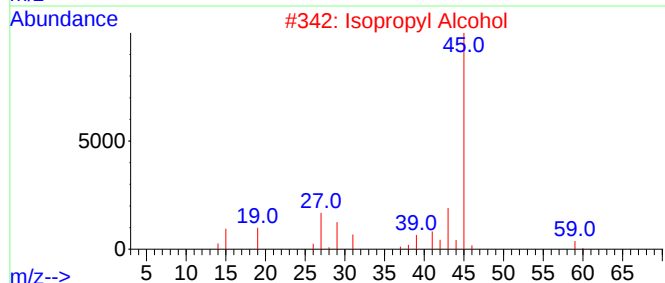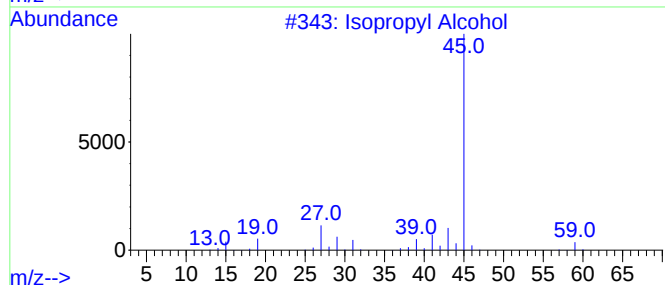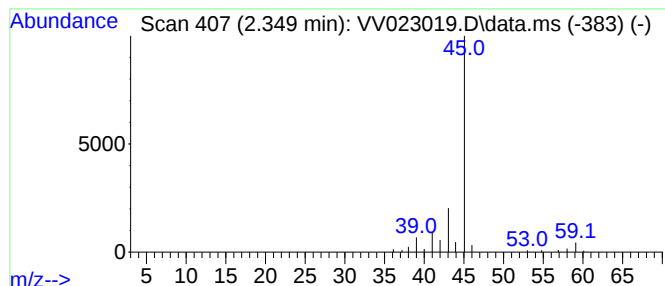

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023019.D
Acq On : 23 Oct 2021 18:59
Operator : SY/MD
Sample : M4277-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.349	1.4	ug/L	73886	1	5.619	260364	5.0