

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023021.D
 Acq On : 23 Oct 2021 19:47
 Operator : SY/MD
 Sample : M4277-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGEO

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023021.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	96	rVB	52999	60145	16.07%	2.403%
2	1.564	155	163	175	rBV	26616	31234	8.34%	1.248%
3	2.098	318	329	340	rBV	63874	87543	23.38%	3.497%
4	2.201	345	361	368	rBV2	9763	27818	7.43%	1.111%
5	2.503	447	455	464	rBV4	4183	6544	1.75%	0.261%
6	3.908	879	892	929	rBV2	70795	225711	60.29%	9.017%
7	4.349	1013	1029	1057	rBV2	43326	110768	29.59%	4.425%
8	5.047	1231	1246	1273	rBV3	101812	253277	67.66%	10.118%
9	5.619	1412	1424	1447	rBV	68066	141878	37.90%	5.668%
10	5.915	1505	1516	1524	rBV9	3256	5761	1.54%	0.230%
11	6.072	1552	1565	1591	rVB2	57071	119615	31.95%	4.779%
12	6.992	1841	1851	1874	rBV2	24636	47855	12.78%	1.912%
13	7.317	1942	1952	1970	rBV	123031	222974	59.56%	8.908%
14	7.400	1972	1978	1995	rVB6	4370	9929	2.65%	0.397%
15	7.629	2040	2049	2068	rBV	18438	34990	9.35%	1.398%
16	7.982	2150	2159	2169	rVB5	6802	11490	3.07%	0.459%
17	8.101	2183	2196	2227	rBV3	140243	374364	100.00%	14.956%
18	8.857	2419	2431	2447	rBV	129790	216671	57.88%	8.656%
19	9.149	2512	2522	2536	rVB7	2826	5634	1.50%	0.225%
20	9.873	2740	2747	2758	rBV4	4369	7805	2.08%	0.312%
21	10.220	2844	2855	2869	rBV	62479	102453	27.37%	4.093%
22	11.252	3166	3176	3191	rBV	118860	185300	49.50%	7.403%
23	11.628	3280	3293	3311	rBV	132544	213368	56.99%	8.524%




Sum of corrected areas: 2503127

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023021.D
Acq On : 23 Oct 2021 19:47
Operator : SY/MD
Sample : M4277-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

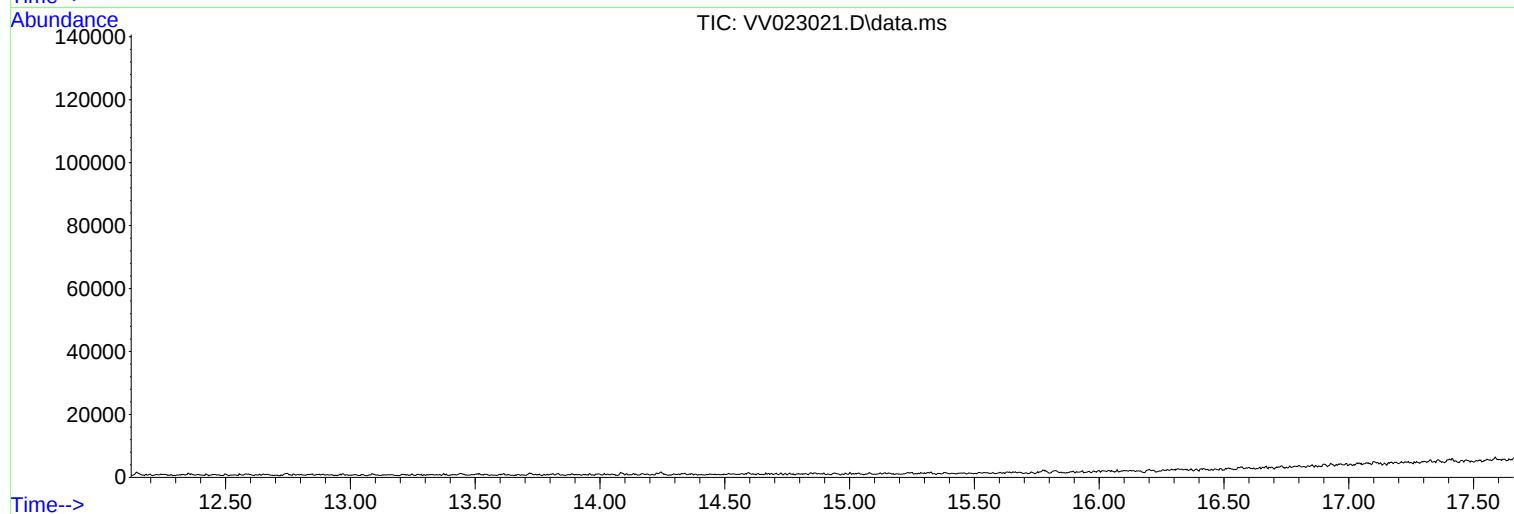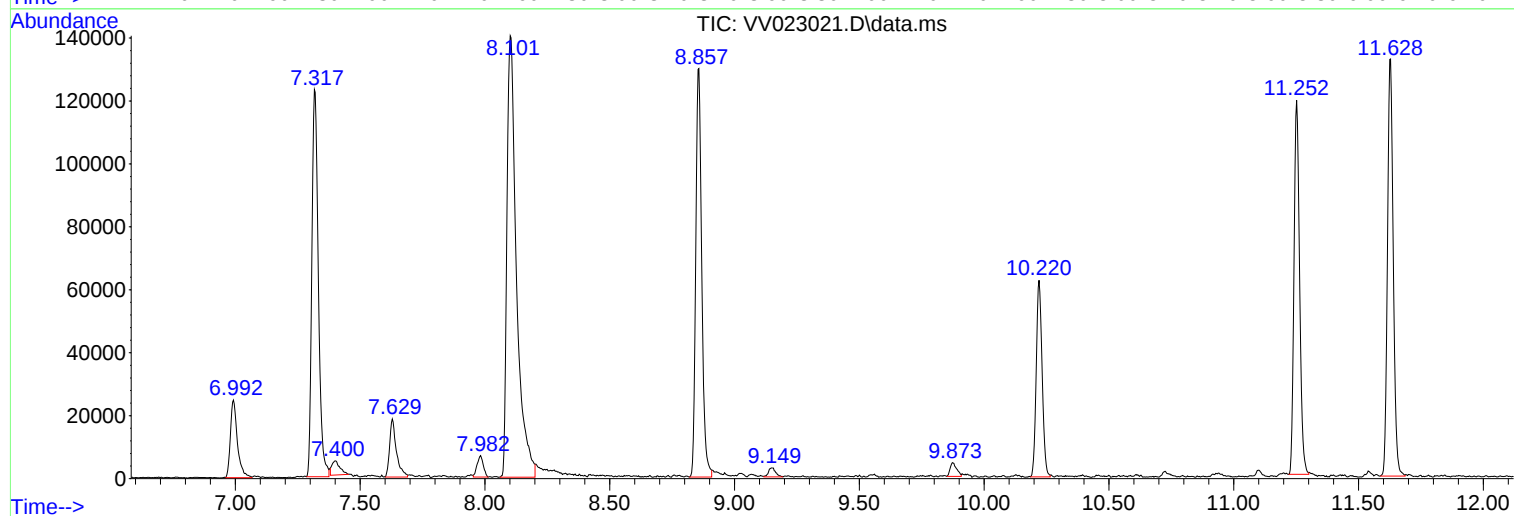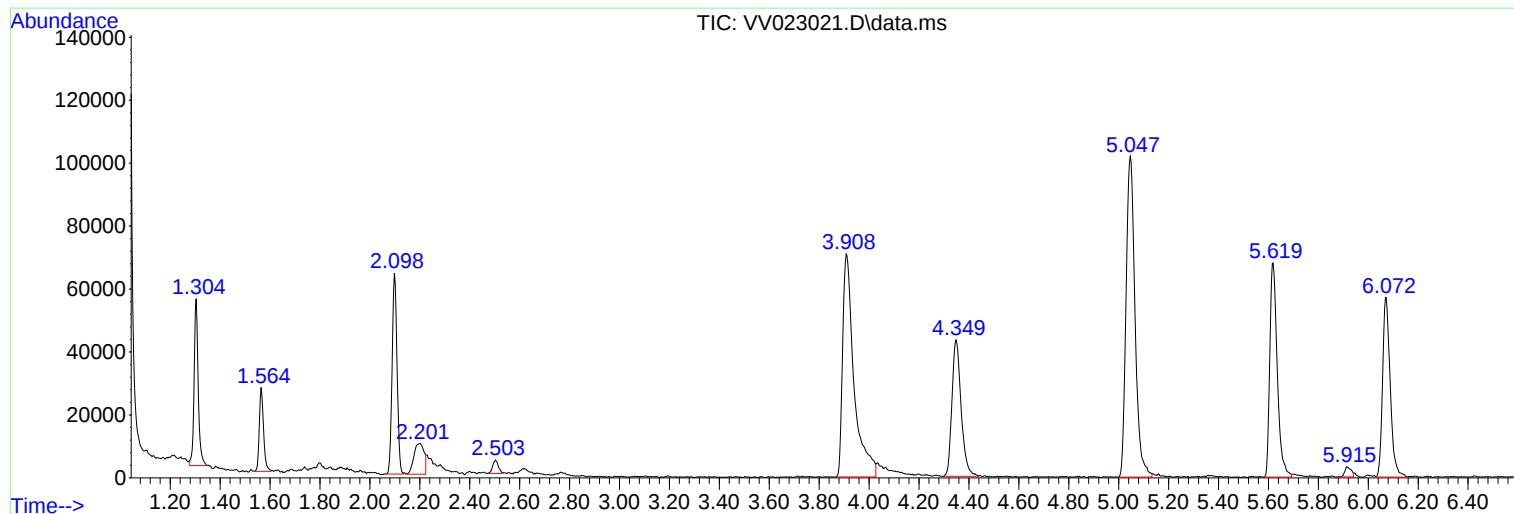

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023021.D
Acq On : 23 Oct 2021 19:47
Operator : SY/MD
Sample : M4277-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023021.D
Acq On : 23 Oct 2021 19:47
Operator : SY/MD
Sample : M4277-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc