

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023022.D
 Acq On : 23 Oct 2021 20:11
 Operator : SY/MD
 Sample : M4277-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGE1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023022.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	92	rVB	55250	59223	13.62%	1.627%
2	1.555	147	160	171	rBV	45702	67086	15.43%	1.843%
3	2.101	319	330	340	rBV	93412	135263	31.12%	3.716%
4	2.166	340	350	377	rVB	249403	434691	100.00%	11.941%
5	2.307	381	394	405	rBV	35635	98655	22.70%	2.710%
6	2.503	448	455	462	rVB2	4690	6912	1.59%	0.190%
7	3.905	874	891	923	rBV3	122353	404155	92.98%	11.102%
8	4.349	1013	1029	1051	rBV	61151	157892	36.32%	4.337%
9	5.047	1231	1246	1273	rBV2	142720	363676	83.66%	9.990%
10	5.619	1412	1424	1448	rBV	89421	190391	43.80%	5.230%
11	5.918	1507	1517	1524	rBV8	2645	4717	1.09%	0.130%
12	6.069	1552	1564	1586	rBV	81274	171738	39.51%	4.718%
13	6.989	1839	1850	1874	rBV2	33261	66026	15.19%	1.814%
14	7.317	1940	1952	1972	rBV	148824	265446	61.07%	7.292%
15	7.397	1972	1977	2000	rVB5	5309	11990	2.76%	0.329%
16	7.625	2039	2048	2066	rBV	19799	39149	9.01%	1.075%
17	8.095	2182	2194	2220	rBV	172861	380798	87.60%	10.461%
18	8.854	2420	2430	2449	rBV	144776	240520	55.33%	6.607%
19	10.220	2840	2855	2868	rBV2	66036	109035	25.08%	2.995%
20	11.252	3165	3176	3195	rBV	125559	201045	46.25%	5.523%
21	11.625	3276	3292	3307	rBV	144300	231858	53.34%	6.369%




Sum of corrected areas: 3640266

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023022.D
Acq On : 23 Oct 2021 20:11
Operator : SY/MD
Sample : M4277-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

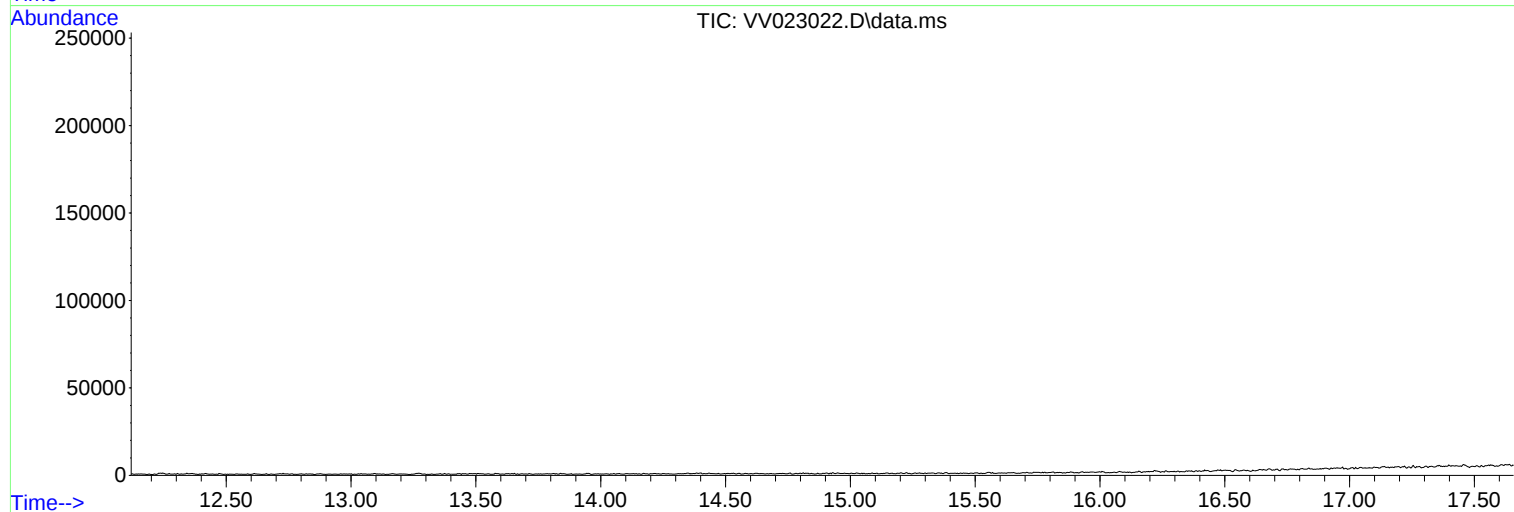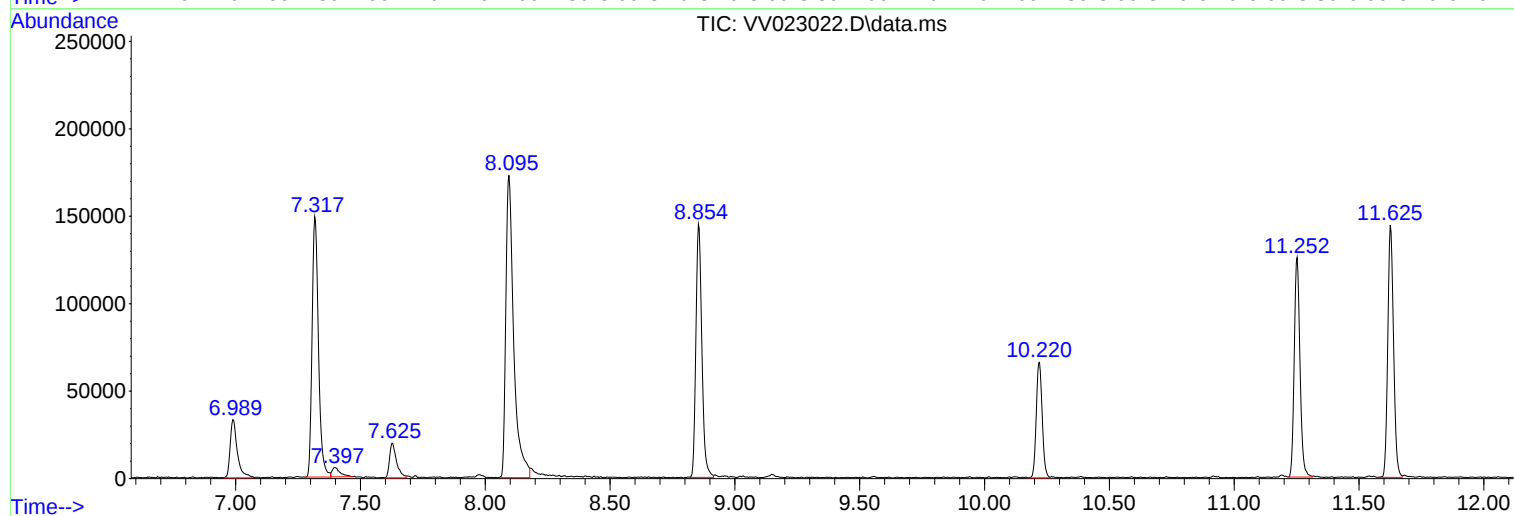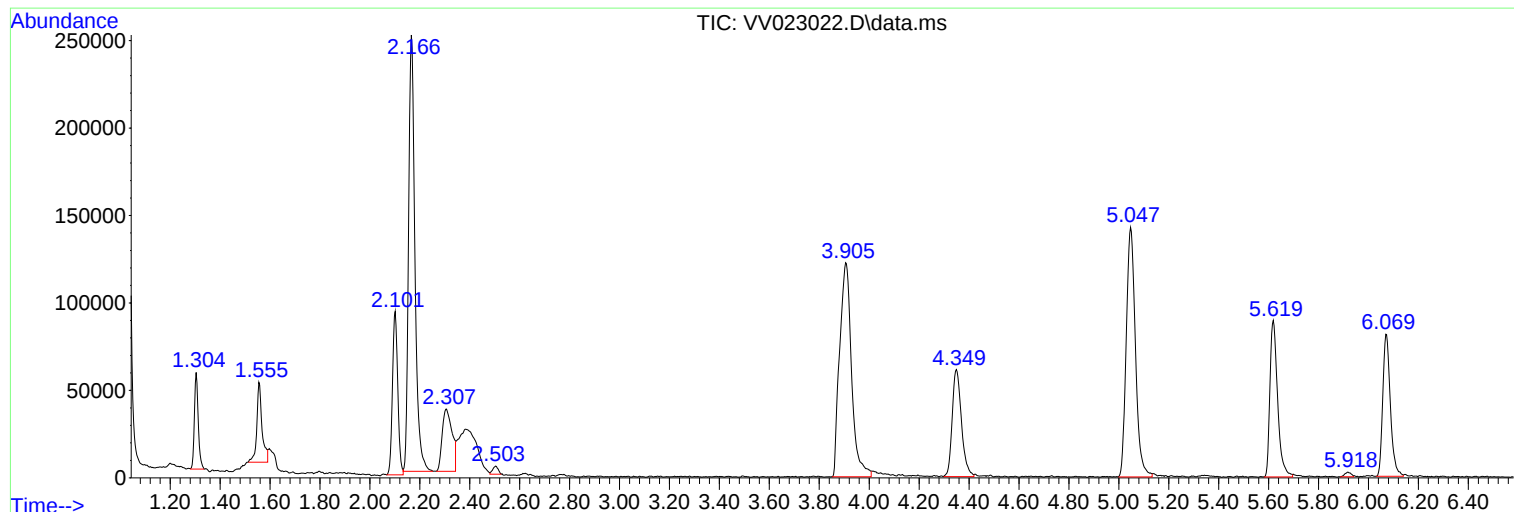

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023022.D
Acq On : 23 Oct 2021 20:11
Operator : SY/MD
Sample : M4277-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE1










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.307	2.59 ug/L	98655	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	72
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	56

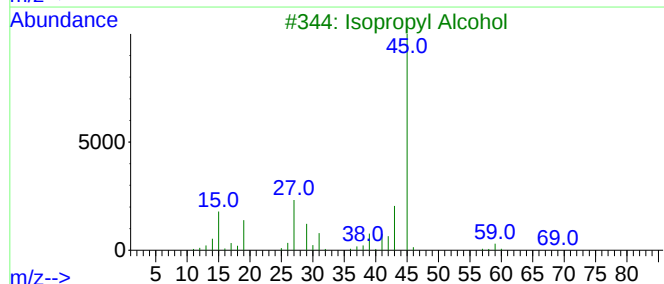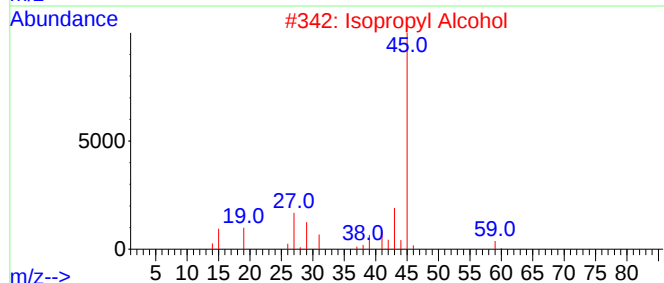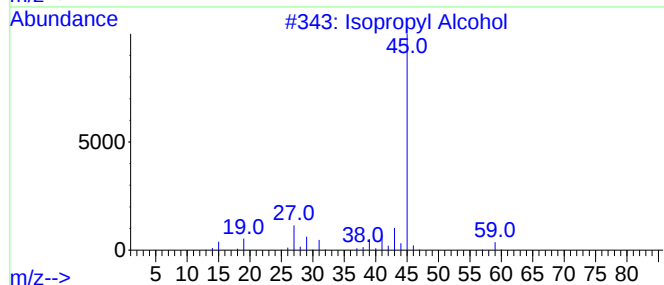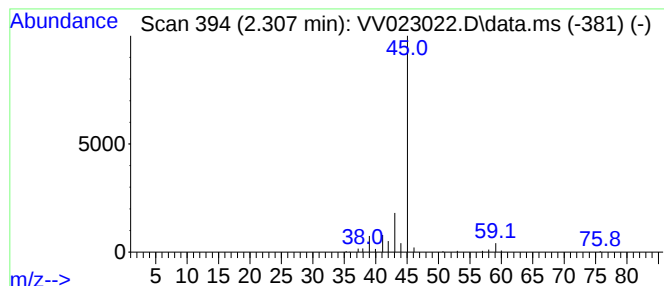

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023022.D
Acq On : 23 Oct 2021 20:11
Operator : SY/MD
Sample : M4277-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.307	2.6	ug/L	98655	1	5.619	190391	5.0