

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023023.D
 Acq On : 23 Oct 2021 20:35
 Operator : SY/MD
 Sample : M4277-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGE2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	58775	63613	16.15%	1.968%
2	1.506	136	145	146	rBV5	3146	4242	1.08%	0.131%
3	1.558	146	161	172	rVV	42634	66530	16.89%	2.058%
4	2.101	319	330	341	rBV	89734	129531	32.88%	4.007%
5	2.169	341	351	375	rVB	82601	150763	38.27%	4.664%
6	2.317	381	397	408	rBV2	20212	64882	16.47%	2.007%
7	2.500	450	454	468	rVB4	5972	10230	2.60%	0.316%
8	2.767	528	537	549	rVB8	1760	4034	1.02%	0.125%
9	3.886	874	885	919	rBV2	56932	203585	51.68%	6.297%
10	4.349	1011	1029	1057	rBV	61074	161827	41.08%	5.006%
11	5.046	1228	1246	1275	rBV2	143309	364285	92.47%	11.268%
12	5.619	1412	1424	1450	rBV	91497	190671	48.40%	5.898%
13	5.918	1507	1517	1533	rBV8	7650	16827	4.27%	0.521%
14	6.072	1551	1565	1587	rBV2	82875	173189	43.96%	5.357%
15	6.989	1840	1850	1871	rBV3	32741	65160	16.54%	2.016%
16	7.316	1941	1952	1970	rBV	148670	264661	67.18%	8.187%
17	7.400	1971	1978	1995	rVB2	5321	11217	2.85%	0.347%
18	7.625	2038	2048	2063	rBV2	19640	36948	9.38%	1.143%
19	7.979	2148	2158	2172	rVB3	41449	72152	18.31%	2.232%
20	8.095	2181	2194	2226	rBV	175265	393967	100.00%	12.186%
21	8.853	2420	2430	2457	rBV	142945	243233	61.74%	7.524%
22	10.220	2842	2855	2871	rBV	68944	111150	28.21%	3.438%
23	11.252	3165	3176	3193	rBV	128364	202625	51.43%	6.268%
24	11.625	3282	3292	3310	rBV	142688	227503	57.75%	7.037%




Sum of corrected areas: 3232825

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV02321\
Data File : VV023023.D
Acq On : 23 Oct 2021 20:35
Operator : SY/MD
Sample : M4277-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

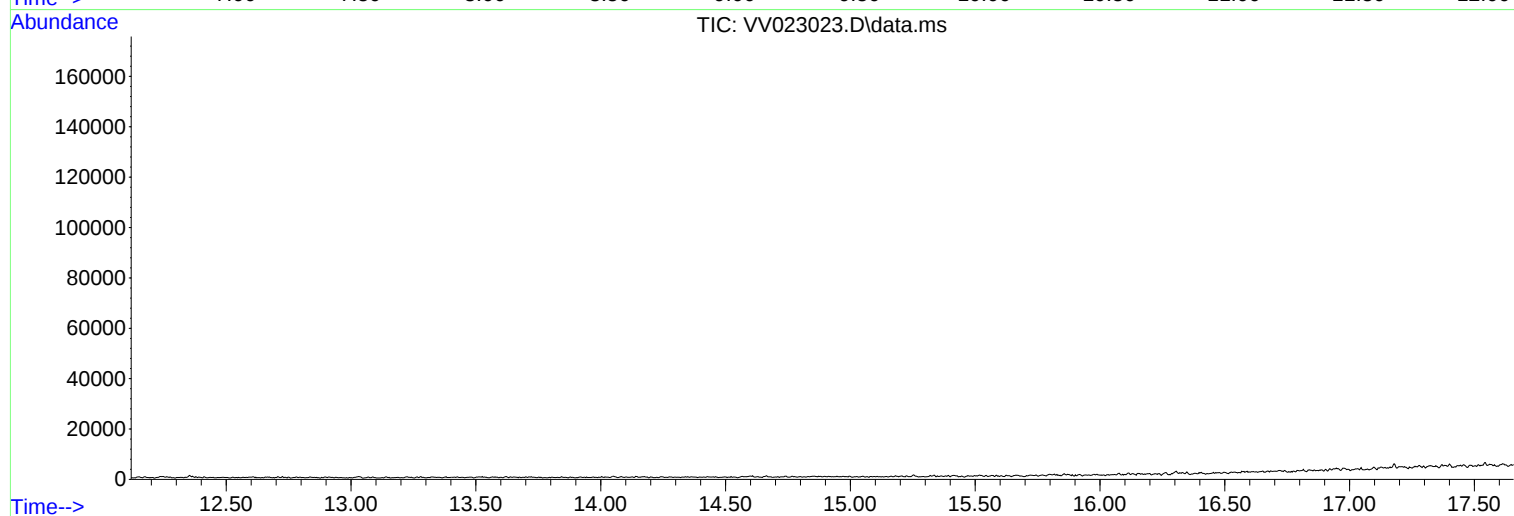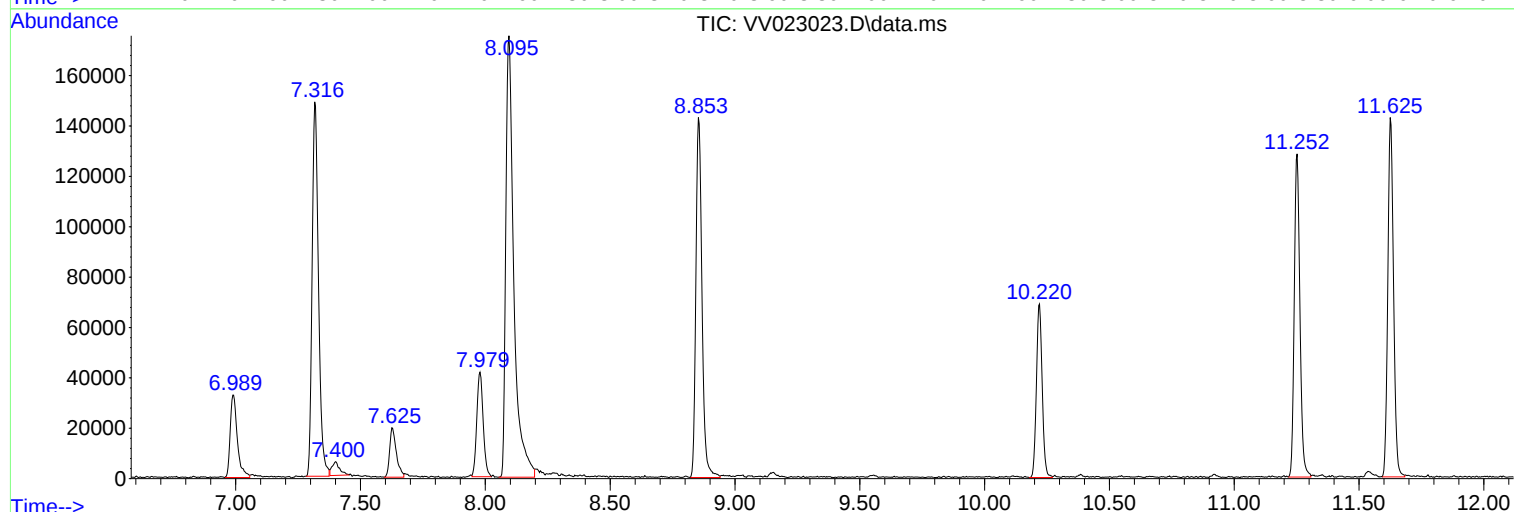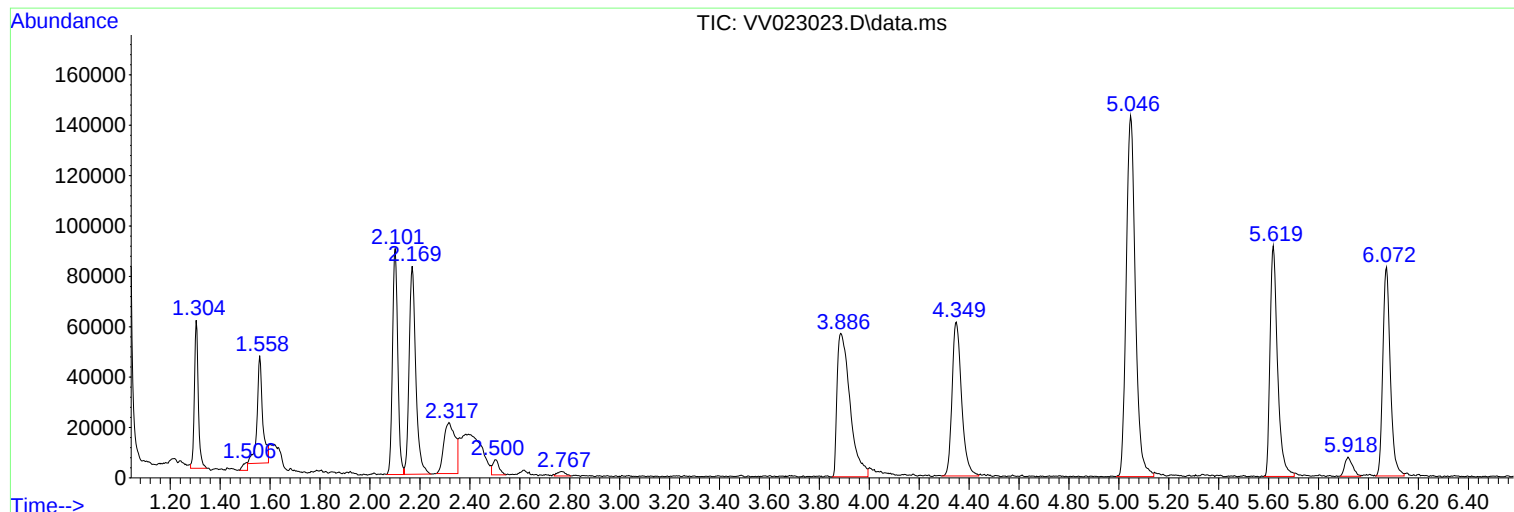

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023023.D
Acq On : 23 Oct 2021 20:35
Operator : SY/MD
Sample : M4277-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE2










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.317	1.70 ug/L	64882	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
3			Formamide	45	CH3NO	000075-12-7	5
4			4-Penten-2-ol	86	C5H10O	000625-31-0	4
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	4

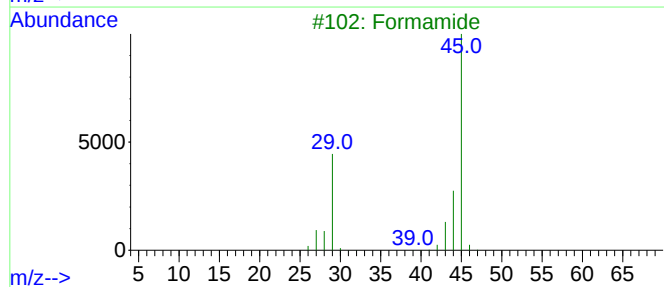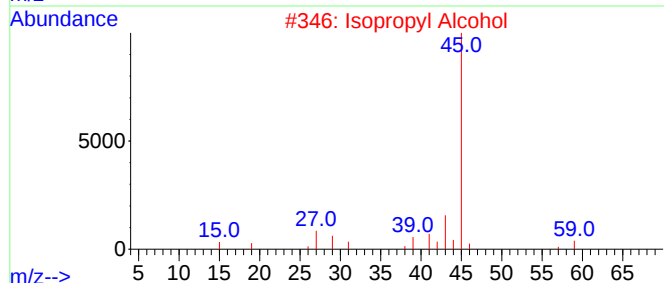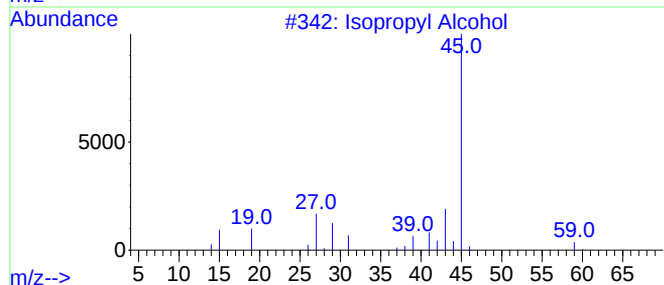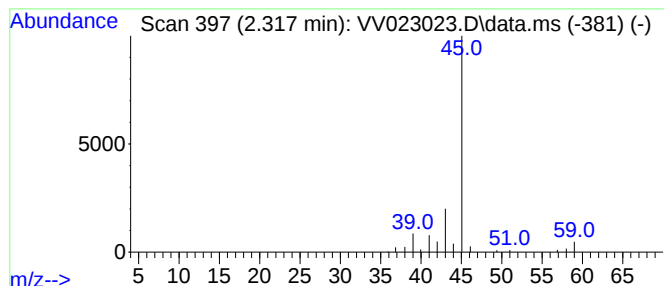

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023023.D
Acq On : 23 Oct 2021 20:35
Operator : SY/MD
Sample : M4277-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.317	1.7	ug/L	64882	1	5.619	190671	5.0