

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023024.D
 Acq On : 23 Oct 2021 20:59
 Operator : SY/MD
 Sample : M4277-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGES

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	31	rVB	11272	11704	2.71%	0.309%
2	1.201	44	50	58	rVB	12194	12312	2.85%	0.325%
3	1.304	75	82	97	rVB	68579	74319	17.18%	1.961%
4	1.561	153	162	172	rVB	43037	50454	11.66%	1.331%
5	2.105	320	331	344	rBV	95752	139186	32.17%	3.672%
6	2.169	345	351	366	rVB	5987	11035	2.55%	0.291%
7	2.317	376	397	410	rBV2	18096	70095	16.20%	1.849%
8	2.503	449	455	465	rVB6	3252	5618	1.30%	0.148%
9	2.767	521	537	554	rBV2	75156	160568	37.11%	4.236%
10	3.741	825	840	856	rBV6	4980	14930	3.45%	0.394%
11	3.883	872	884	916	rBV2	61950	188258	43.51%	4.966%
12	4.349	1009	1029	1064	rBV2	70607	186421	43.09%	4.918%
13	5.047	1231	1246	1271	rBV2	157187	399640	92.37%	10.542%
14	5.619	1413	1424	1448	rBV	106057	218646	50.53%	5.768%
15	5.921	1506	1518	1533	rBV	6968	16544	3.82%	0.436%
16	6.072	1549	1565	1584	rBV	92375	193019	44.61%	5.092%
17	6.989	1840	1850	1871	rBV2	37516	72521	16.76%	1.913%
18	7.320	1941	1953	1970	rBV	168442	300002	69.34%	7.914%
19	7.397	1972	1977	1986	rVB5	5029	8570	1.98%	0.226%
20	7.625	2040	2048	2069	rBV	22921	41889	9.68%	1.105%
21	7.976	2143	2157	2171	rBV	180621	298864	69.08%	7.884%
22	8.092	2183	2193	2232	rBV	218605	432663	100.00%	11.413%
23	8.854	2418	2430	2456	rBV	169221	281936	65.16%	7.437%
24	10.217	2841	2854	2870	rBV	77953	122762	28.37%	3.238%
25	11.249	3165	3175	3202	rVB	146175	227022	52.47%	5.989%
26	11.625	3281	3292	3310	rBV	158673	251824	58.20%	6.643%




Sum of corrected areas: 3790802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023024.D
Acq On : 23 Oct 2021 20:59
Operator : SY/MD
Sample : M4277-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

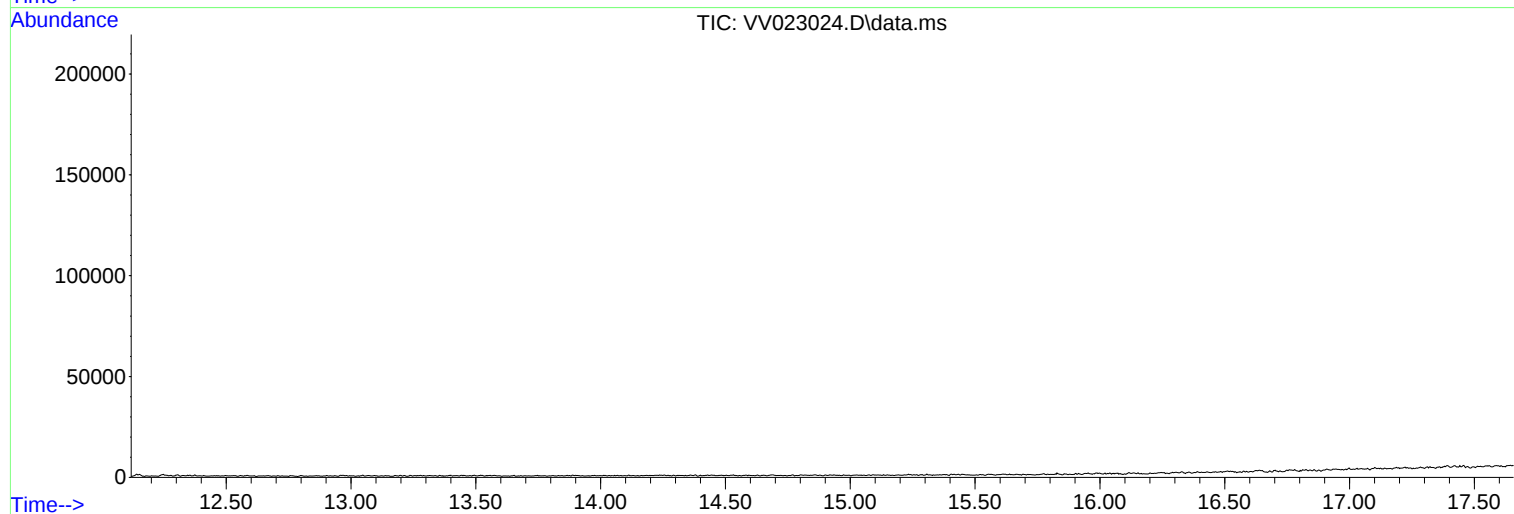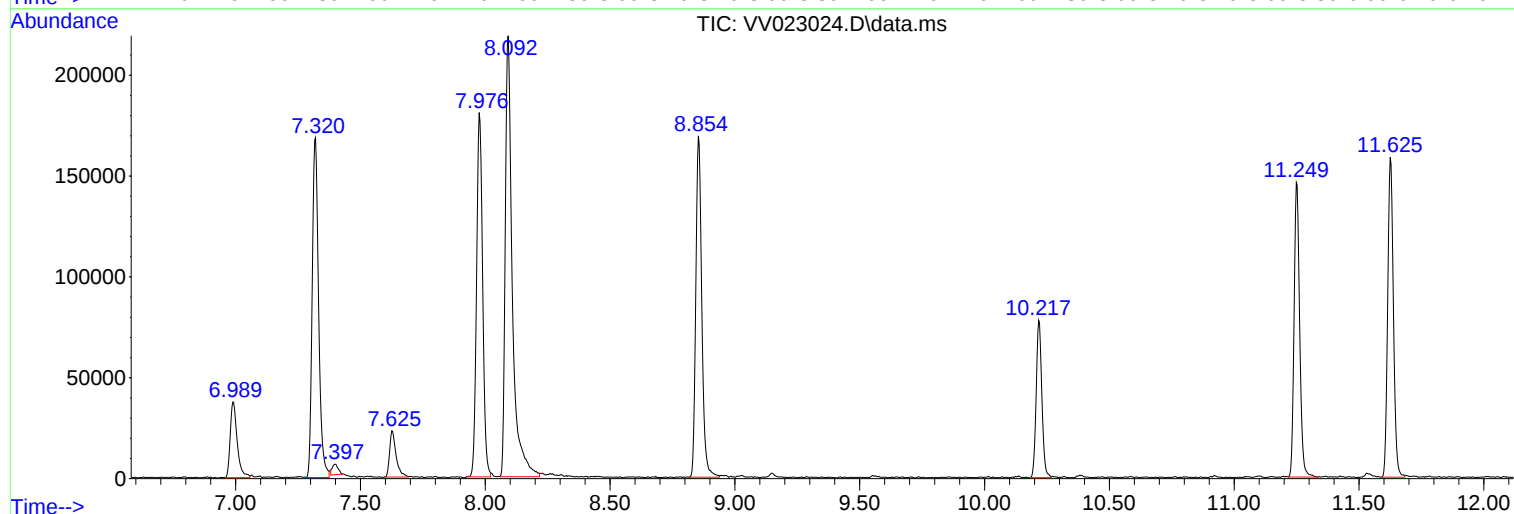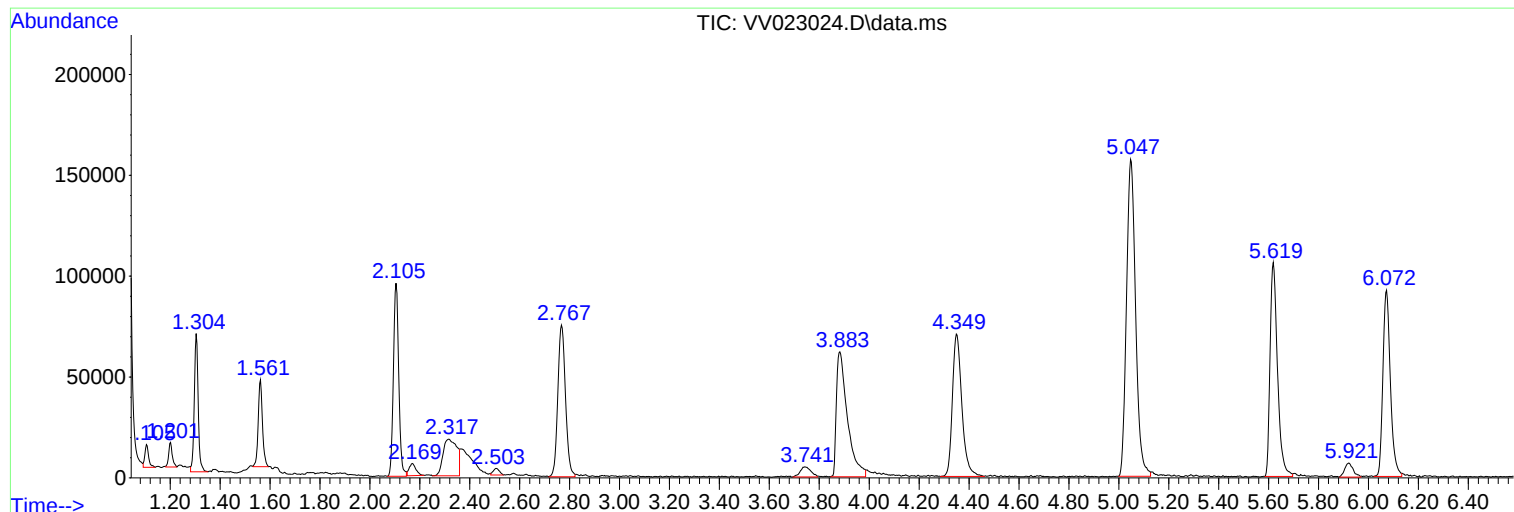

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023024.D
Acq On : 23 Oct 2021 20:59
Operator : SY/MD
Sample : M4277-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.317	1.60 ug/L	70095	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
2			Formamide	45	CH3NO	000075-12-7	4
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	4
4			1-Butene, 4-methoxy	86	C5H10O	004696-30-4	4
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	4

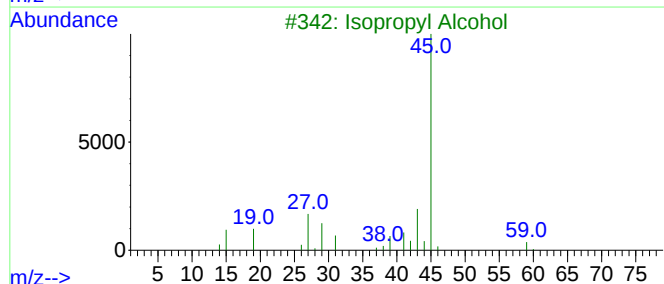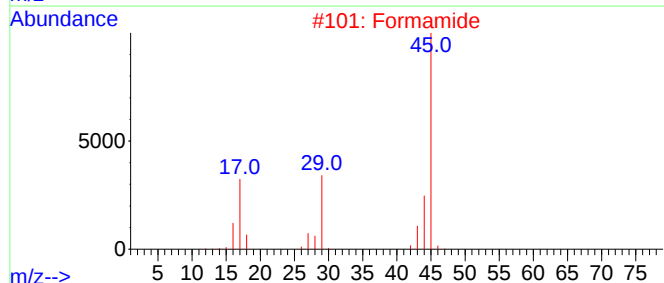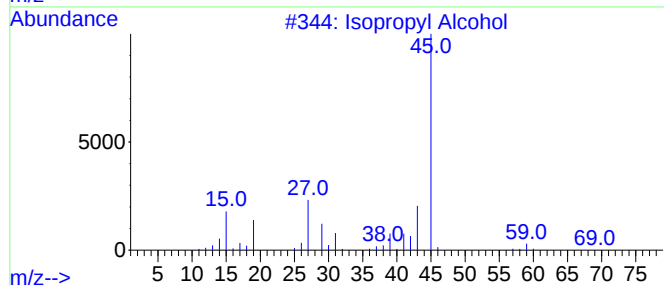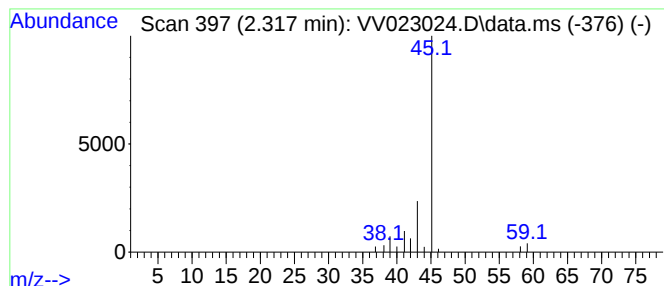

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
Data File : VV023024.D
Acq On : 23 Oct 2021 20:59
Operator : SY/MD
Sample : M4277-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	2.317	1.6	ug/L	70095	1	5.619	218646	5.0