


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102321\
 Data File : VV023002.D
 Acq On : 23 Oct 2021 10:40
 Operator : SY/MD
 Sample : BFB221
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB221

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Oct 28 01:43:46 2021

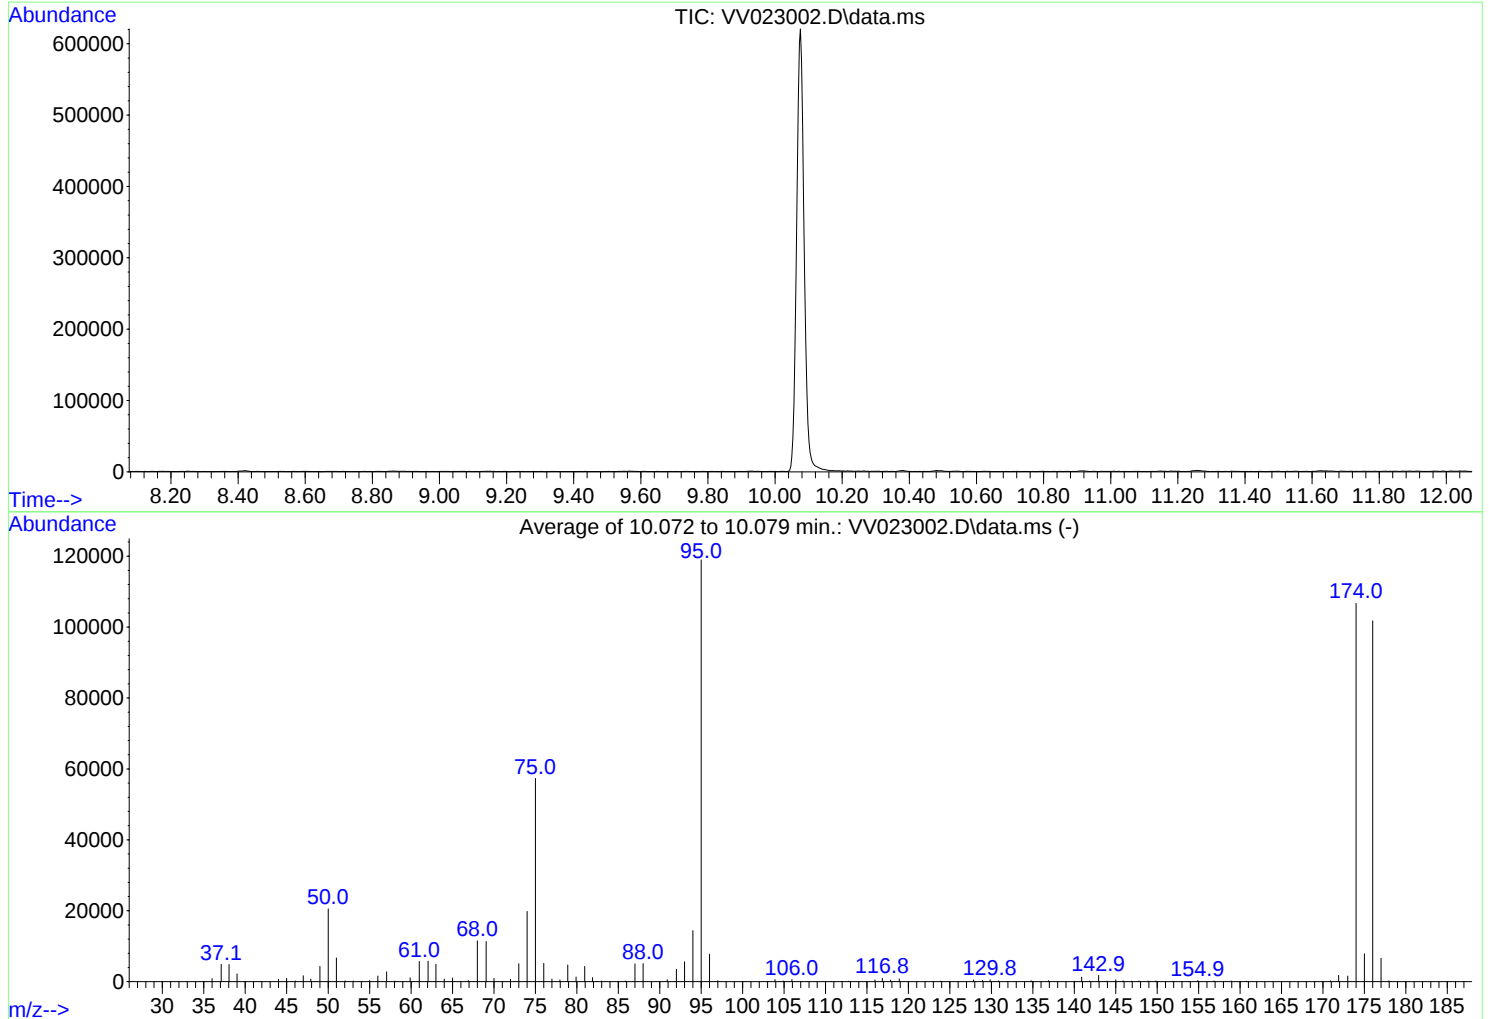

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	20544	PASS
75	95	30	80	48.2	57304	PASS
95	95	100	100	100.0	118973	PASS
96	95	5	9	6.5	7779	PASS
173	174	0.00	2	1.5	1600	PASS
174	95	50	120	89.7	106693	PASS
175	174	5	9	7.4	7858	PASS
176	174	95	105	95.4	101760	PASS
177	176	5	10	6.5	6615	PASS

m/z	Abundance
36.00	824.0
37.10	4527.0
38.00	4647.0
39.00	2098.0
39.90	245.0
44.00	795.0
45.00	957.0
46.00	162.0
47.00	1521.0
47.90	523.0
48.00	528.0
49.00	4100.0
50.00	19208.0
51.00	6166.0
52.00	242.0
53.10	229.0
55.00	306.0
56.00	1367.0
57.00	2615.0
58.00	145.0
59.90	1031.0
61.00	5360.0
62.10	5642.0
63.00	4603.0
64.00	735.0
65.00	1008.0
66.00	135.0
66.90	280.0
68.00	10705.0
69.10	10564.0
70.00	880.0
71.00	109.0
72.00	643.0
73.00	4686.0
74.00	18552.0
75.00	54480.0
76.00	4806.0
77.00	639.0
78.00	495.0
78.90	4414.0
79.90	1295.0
81.00	4133.0
81.90	996.0
83.00	168.0
85.80	219.0
87.00	4902.0
88.00	4824.0
90.90	508.0
92.00	3160.0
93.00	5312.0
94.00	13858.0
95.00	113200.0
96.00	7221.0
97.00	268.0
103.90	508.0
104.90	183.0
105.90	566.0
107.20	119.0
107.80	101.0
110.70	119.0
111.90	113.0
112.80	116.0
115.00	125.0
116.00	466.0
116.80	960.0
117.80	417.0
118.90	757.0
123.80	121.0
127.90	503.0
129.00	339.0
129.90	474.0
130.80	214.0
134.80	250.0
136.90	289.0
140.10	142.0
140.90	1318.0
141.90	172.0
143.00	1545.0
143.90	195.0
145.00	476.0
145.90	225.0
146.90	138.0
147.80	262.0
148.90	154.0
149.90	176.0
153.00	140.0
153.80	103.0
154.90	283.0
156.80	284.0
159.00	144.0
160.80	130.0
170.90	234.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

171.90	1860.0
173.00	1503.0
174.00	105256.0
175.00	7371.0
176.00	100424.0
177.00	6291.0
177.90	207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

Scan 2796 (10.030 min): VV023002.D\data.ms
BFB221

m/z	Abundance
39.80	191.0
44.00	192.0
50.70	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

m/z	Abundance
36.00	877.0
37.10	4997.0
38.10	4847.0
39.00	2147.0
40.00	262.0
41.90	115.0
44.00	830.0
45.00	949.0
46.00	230.0
47.00	1706.0
47.90	536.0
49.00	4339.0
50.00	21064.0
51.00	6970.0
52.10	246.0
53.00	162.0
55.00	328.0
56.00	1738.0
57.10	2871.0
58.10	218.0
59.90	1156.0
61.00	5761.0
62.00	5706.0
63.00	5020.0
64.00	733.0
65.00	1022.0
65.90	166.0
66.90	342.0
68.00	11798.0
69.00	11716.0
70.00	923.0
72.00	662.0
73.00	5228.0
74.00	20432.0
75.00	58120.0
76.00	5263.0
77.00	742.0
77.90	501.0
78.90	4834.0
79.90	1266.0
80.90	4288.0
81.90	1210.0
83.00	156.0
85.90	168.0
87.00	5027.0
88.00	5253.0
90.90	593.0
92.00	3673.0
93.00	5773.0
94.00	14440.0
95.00	120752.0
96.00	8147.0
97.00	258.0
102.90	103.0
103.90	627.0
104.90	181.0
106.00	591.0
112.80	120.0
115.90	526.0
116.90	909.0
117.90	485.0
118.90	784.0
123.90	126.0
127.80	493.0
128.90	297.0
129.80	572.0
130.90	244.0
134.80	268.0
136.90	271.0
140.00	160.0
140.90	1207.0
141.80	156.0
142.90	1884.0
144.00	159.0
145.00	510.0
145.90	258.0
146.90	103.0
147.80	217.0
148.90	191.0
149.80	251.0
151.80	119.0
153.80	123.0
154.90	313.0
156.90	207.0
158.90	186.0
160.80	180.0
170.90	251.0
171.90	1645.0
173.00	1613.0
174.00	104160.0
175.00	8118.0
176.00	99216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

177.006738.0

178.00227.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

m/z	Abundance
36.00	880.0
37.10	5061.0
38.10	5067.0
39.00	2238.0
40.00	255.0
41.90	111.0
44.00	832.0
45.00	950.0
46.10	209.0
47.00	1746.0
47.80	548.0
49.00	4371.0
50.00	21360.0
51.00	6932.0
52.00	250.0
53.10	215.0
55.00	331.0
56.00	1626.0
57.00	2788.0
58.10	189.0
59.90	1114.0
61.00	5882.0
62.10	6003.0
63.00	5115.0
64.00	738.0
65.00	1038.0
66.00	160.0
66.90	320.0
68.00	11982.0
69.00	11656.0
70.00	931.0
72.00	702.0
73.00	5214.0
74.00	20504.0
75.00	59312.0
76.00	5309.0
77.00	755.0
78.00	518.0
78.90	4829.0
79.90	1315.0
81.00	4415.0
81.90	1215.0
83.00	177.0
85.80	200.0
87.00	5168.0
88.00	5239.0
90.90	549.0
92.00	3598.0
93.00	5744.0
94.00	14942.0
95.00	122968.0
96.00	7969.0
97.00	294.0
103.90	619.0
104.90	187.0
105.90	610.0
107.80	107.0
110.70	102.0
112.80	132.0
115.00	111.0
116.00	534.0
116.80	949.0
117.80	475.0
118.90	826.0
123.90	132.0
127.80	526.0
128.90	336.0
129.80	574.0
130.90	237.0
134.80	275.0
136.90	309.0
140.10	170.0
140.90	1327.0
141.80	176.0
143.00	1805.0
143.90	208.0
145.00	526.0
145.90	249.0
146.90	140.0
147.80	252.0
148.90	194.0
149.80	223.0
151.80	131.0
153.00	115.0
153.80	120.0
154.90	339.0
156.90	255.0
158.90	174.0
160.80	165.0
170.90	266.0
171.90	1848.0
173.00	1685.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

174.00	110664.0
175.00	8085.0
176.00	105640.0
177.00	6815.0
178.00	241.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221