




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032575.D
Acq On : 23 Oct 2023 17:05
Operator : SY/MD
Sample : 05043-01DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B19DL

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/26/2023
Supervised By :Semsettin Yesilyurt 10/26/2023

Quant Time: Oct 24 04:48:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 21 02:44:24 2023
Response via : Initial Calibration

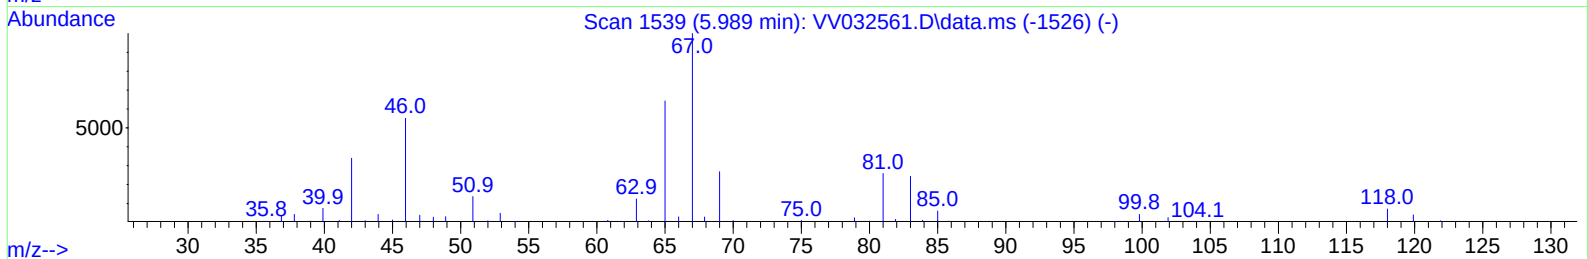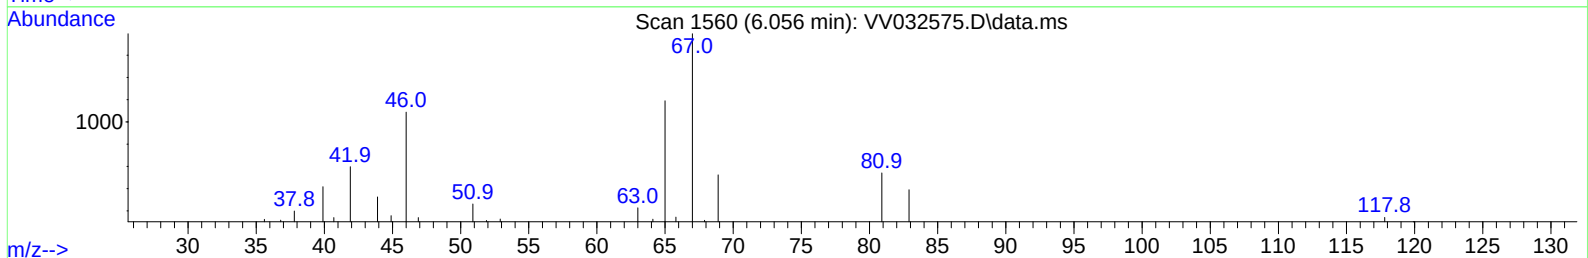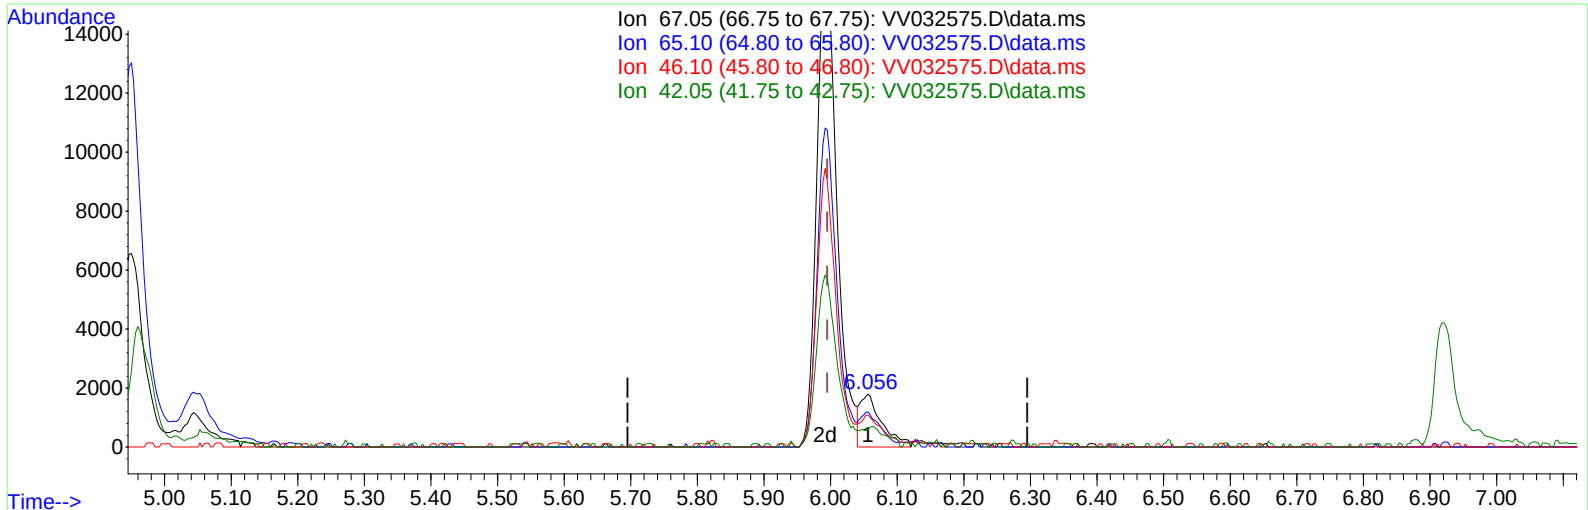

TIC: VV032575.D\data.ms

(36) 1,2-Dichloropropane-d6 (S)

6.056min (+ 0.061) 0.41 ug/L

response 4015

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	67.60	52.48
46.10	49.60	50.61
42.05	26.30	33.03




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032575.D
Acq On : 23 Oct 2023 17:05
Operator : SY/MD
Sample : 05043-01DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B19DL

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/26/2023
Supervised By :Semsettin Yesilyurt 10/26/2023

Quant Time: Oct 24 04:48:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 21 02:44:24 2023
Response via : Initial Calibration

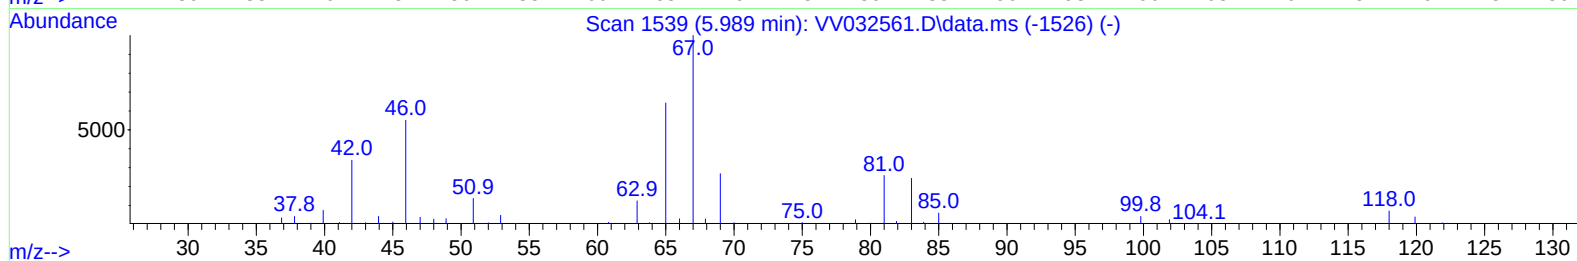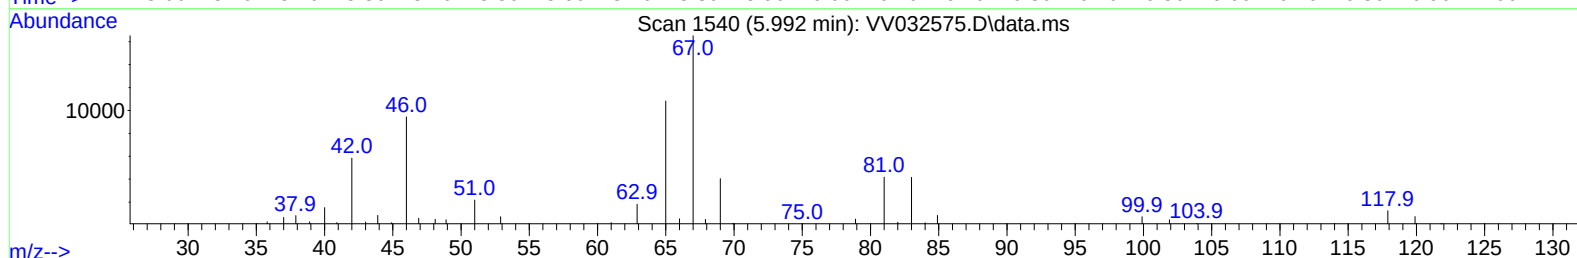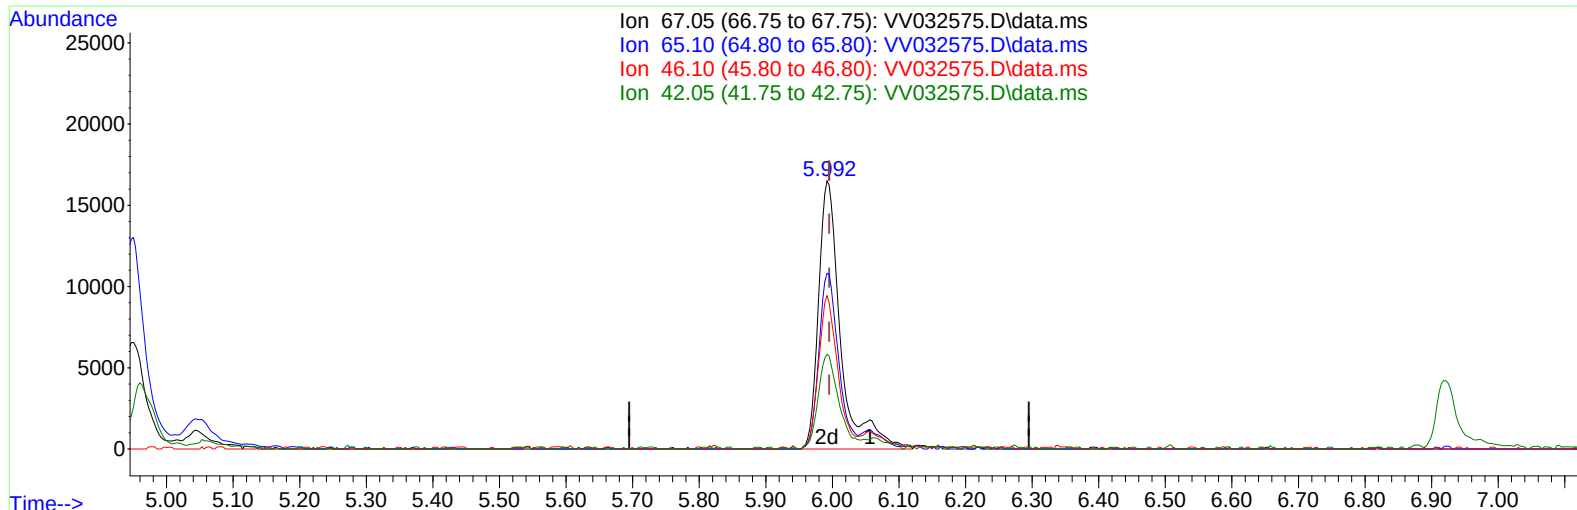

TIC: VV032575.D\data.ms

(36) 1,2-Dichloropropane-d6 (S)

5.992min (-0.003) 3.92 ug/L m

response 38324

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	67.60	5.50#
46.10	49.60	5.30#
42.05	26.30	3.46#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102323\
 Data File : VW032575.D
 Acq On : 23 Oct 2023 17:05
 Operator : SY/MD
 Sample : 05043-01DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B19DL

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/26/2023
 Supervised By :Semsettin Yesilyurt 10/26/2023

Quant Time: Oct 24 04:48:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 21 02:44:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	84891	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	100208	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	41557	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	24806	3.593	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	71.800%	
7) Chloroethane-d5	1.532	69	25103	4.479	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	89.600%	
11) 1,1-Dichloroethene-d2	2.056	65	9838	3.379	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.600%	
20) 2-Butanone-d5	3.825	46	89877	51.461	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	102.920%	
24) Chloroform-d	4.252	84	51557	4.233	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	84.600%	
26) 1,2-Dichloroethane-d4	4.950	65	29929	5.188	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.800%	
32) Benzene-d6	4.963	84	94431	3.203	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	64.000%#	
36) 1,2-Dichloropropane-d6	5.992	67	38324m	3.923	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	78.400%	
41) Toluene-d8	7.246	98	79109	2.934	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	58.600%#	
43) trans-1,3-Dichloroprop...	7.561	79	12518	3.616	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	72.400%	
46) 2-Hexanone-d5	8.034	63	79401	48.748	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	97.500%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	34163	5.000	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	100.000%	
66) 1,2-Dichlorobenzene-d4	11.564	152	33300	4.318	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	86.400%	
Target Compounds						
16) Methylene chloride	2.449	84	2311	0.285	ug/L	86
47) Tetrachloroethene	7.908	164	29380	4.022	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032575.D
Acq On : 23 Oct 2023 17:05
Operator : SY/MD
Sample : 05043-01DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B19DL

Manual IntegrationsAPPROVED

Quant Time: Oct 24 04:48:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 21 02:44:24 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/26/2023
Supervised By :Semsettin Yesilyurt 10/26/2023

