




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
 Data File : VV032577.D
 Acq On : 23 Oct 2023 17:53
 Operator : SY/MD
 Sample : 04994-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B26

Manual Integrations APPROVED

Quant Time: Oct 24 04:48:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 21 02:44:24 2023
 Response via : Initial Calibration

Reviewed By : John Carlone 10/24/2023
 Supervised By : Mahesh Dadoda 10/26/2023

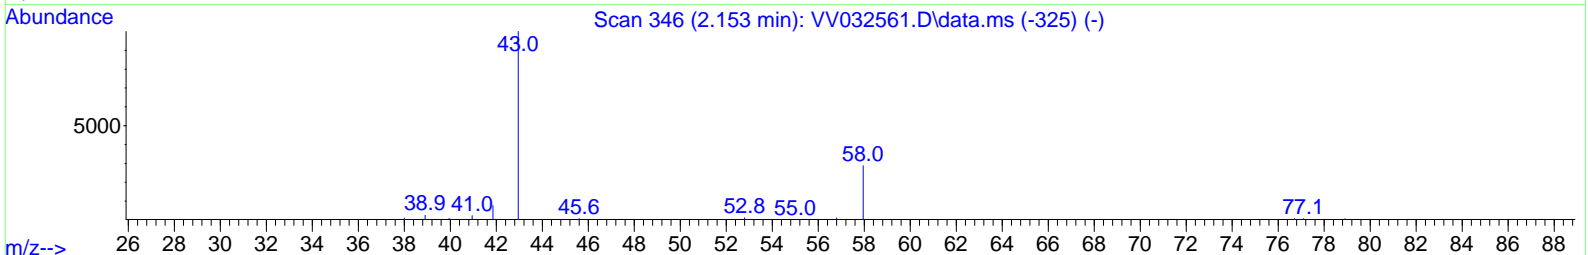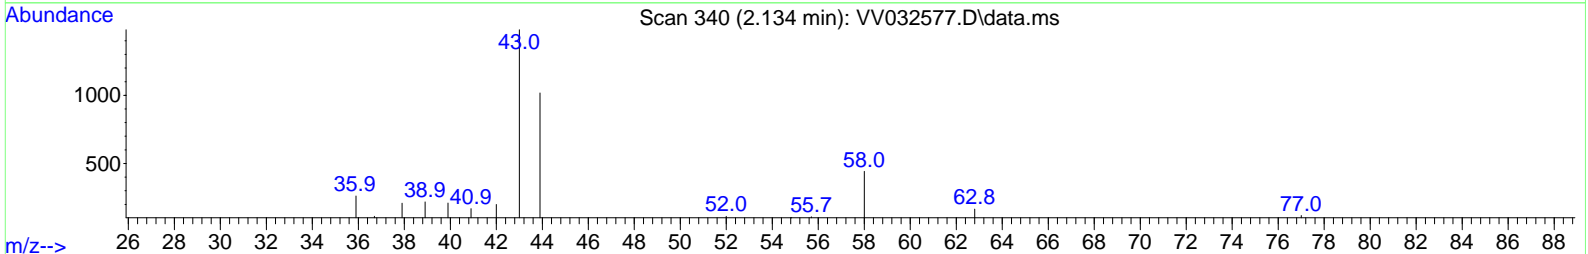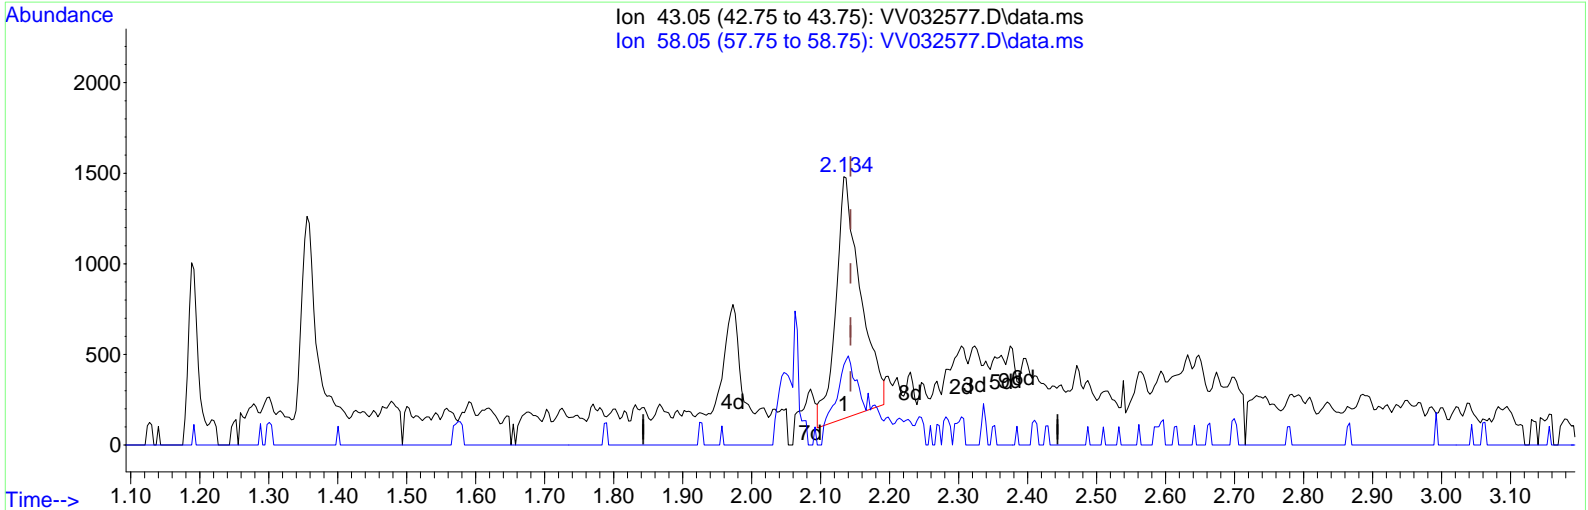

TIC: VV032577.D\data.ms

(13) Acetone (T)

2.134min (-0.010) 2.39 ug/L

response	3288
Ion	Exp% Act%
43.05	100.00 100.00
58.05	33.00 35.04
0.00	0.00 0.00
0.00	0.00 0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
 Data File : VV032577.D
 Acq On : 23 Oct 2023 17:53
 Operator : SY/MD
 Sample : 04994-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 C0B26

Manual IntegrationsAPPROVED

Quant Time: Oct 24 04:48:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 21 02:44:24 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/24/2023
 Supervised By :Mahesh Dadoda 10/26/2023

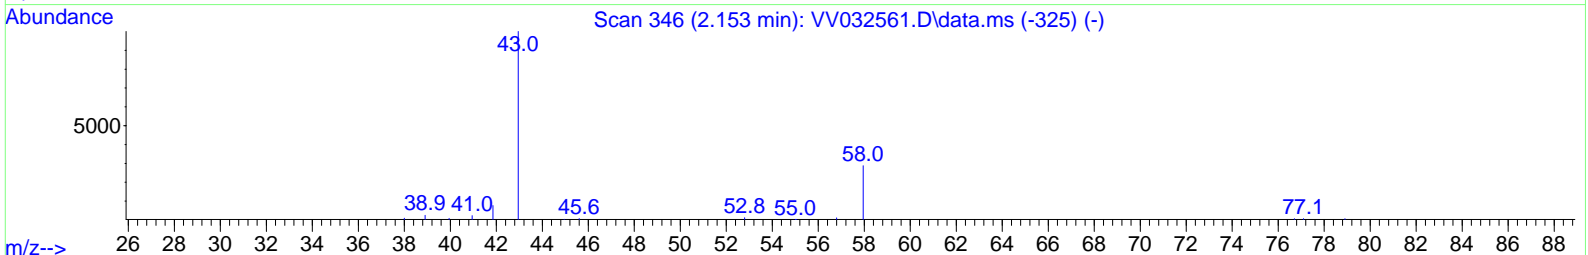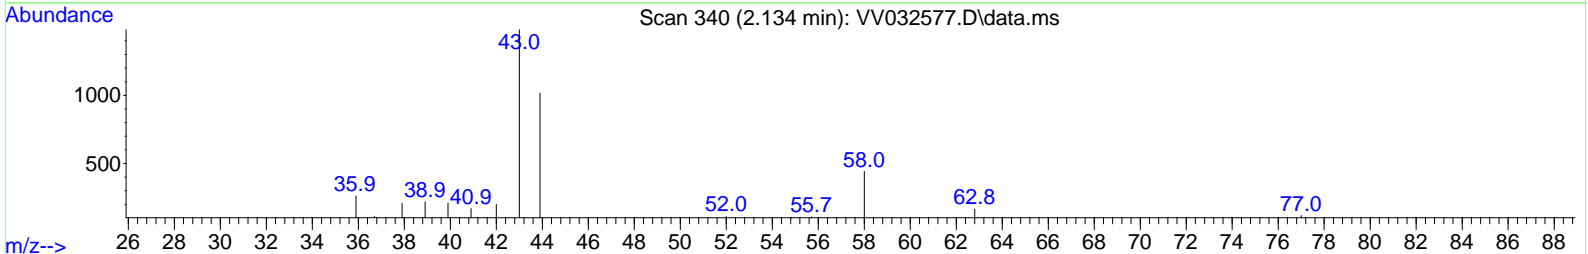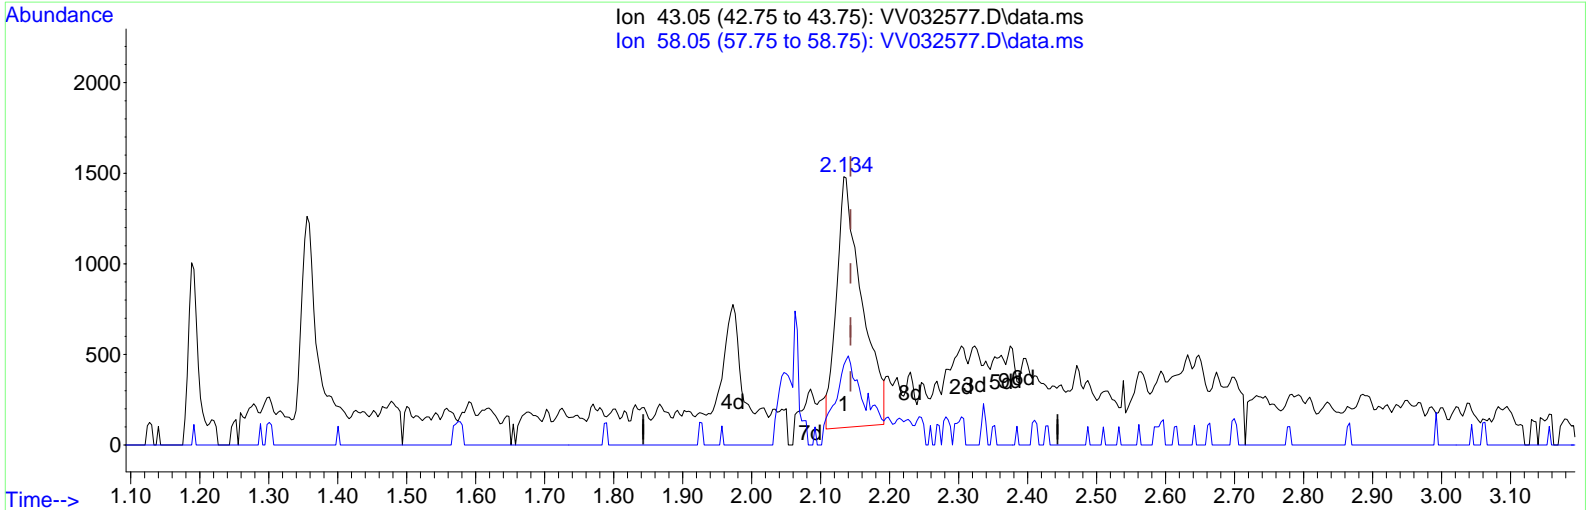

TIC: VV032577.D\data.ms

(13) Acetone (T)

2.134min (-0.010) 2.55 ug/L m

response	3504
Ion	Exp% Act%
43.05	100.00 100.00
58.05	33.00 32.88
0.00	0.00 0.00
0.00	0.00 0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102323\
 Data File : VW032577.D
 Acq On : 23 Oct 2023 17:53
 Operator : SY/MD
 Sample : 04994-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 C0B26

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/24/2023
 Supervised By :Mahesh Dadoda 10/26/2023

Quant Time: Oct 24 04:48:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 21 02:44:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	86765	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	100961	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	42835	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	24952	3.536	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	70.800%	
7) Chloroethane-d5	1.532	69	26451	4.618	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	92.400%	
11) 1,1-Dichloroethene-d2	2.060	65	10209	3.430	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.600%	
20) 2-Butanone-d5	3.809	46	72015	40.343	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	80.680%	
24) Chloroform-d	4.252	84	60747	4.880	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.600%	
26) 1,2-Dichloroethane-d4	4.947	65	32267	5.472	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	109.400%	
32) Benzene-d6	4.963	84	100133	3.371	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	67.400%#	
36) 1,2-Dichloropropane-d6	5.992	67	35603	3.617	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	72.400%	
41) Toluene-d8	7.246	98	83880	3.088	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	61.800%#	
43) trans-1,3-Dichloroprop...	7.558	79	12078	3.463	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	69.200%	
46) 2-Hexanone-d5	8.030	63	77166	47.022	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.040%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	33795	4.909	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	98.200%	
66) 1,2-Dichlorobenzene-d4	11.564	152	34160	4.298	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	86.000%	
Target Compounds						
13) Acetone	2.134	43	3504m	2.547	ug/L	
25) Chloroform	4.278	83	107430	7.986	ug/L	98
38) Bromodichloromethane	6.439	83	25041	2.217	ug/L #	99
49) Dibromochloromethane	8.182	129	4870	0.698	ug/L	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
 Data File : VV032577.D
 Acq On : 23 Oct 2023 17:53
 Operator : SY/MD
 Sample : 04994-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 C0B26

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/24/2023
 Supervised By :Mahesh Dadoda 10/26/2023

Quant Time: Oct 24 04:48:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 21 02:44:24 2023
 Response via : Initial Calibration

