

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
 Data File : VV032562.D
 Acq On : 23 Oct 2023 11:43
 Operator : SY/MD
 Sample : VV1023WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK376

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032562.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	8	21	31	rVB	4366	9454	1.78%	0.274%
2	1.275	67	73	88	rVB	51747	57388	10.78%	1.662%
3	1.532	144	153	163	rBV	52140	63474	11.92%	1.838%
4	2.060	306	317	331	rBV	79907	118416	22.25%	3.430%
5	2.172	341	352	364	rVB2	8531	18106	3.40%	0.524%
6	3.822	854	865	905	rBV2	35492	170331	32.00%	4.933%
7	4.253	984	999	1020	rBV	62885	163418	30.70%	4.733%
8	4.359	1023	1032	1055	rVB2	8456	25075	4.71%	0.726%
9	4.960	1202	1219	1236	rBV3	146584	375319	70.51%	10.871%
10	5.535	1388	1398	1414	rBV	117086	241566	45.38%	6.997%
11	5.603	1414	1419	1437	rVB2	9732	25247	4.74%	0.731%
12	5.992	1528	1540	1554	rBV2	90912	192965	36.25%	5.589%
13	6.918	1817	1828	1850	rBV	41387	85746	16.11%	2.484%
14	7.246	1919	1930	1955	rBV	148121	288927	54.28%	8.368%
15	7.561	2015	2028	2053	rBV2	24375	55113	10.35%	1.596%
16	8.031	2163	2174	2219	rBV	232958	532279	100.00%	15.417%
17	8.786	2398	2409	2431	rBV	188088	337751	63.45%	9.783%
18	10.156	2823	2835	2851	rBV	79810	129694	24.37%	3.756%
19	11.188	3144	3156	3175	rBV	180555	289122	54.32%	8.374%
20	11.564	3259	3273	3292	rBV	167198	273194	51.33%	7.913%




Sum of corrected areas: 3452585

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032562.D
Acq On : 23 Oct 2023 11:43
Operator : SY/MD
Sample : VV1023WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK376

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

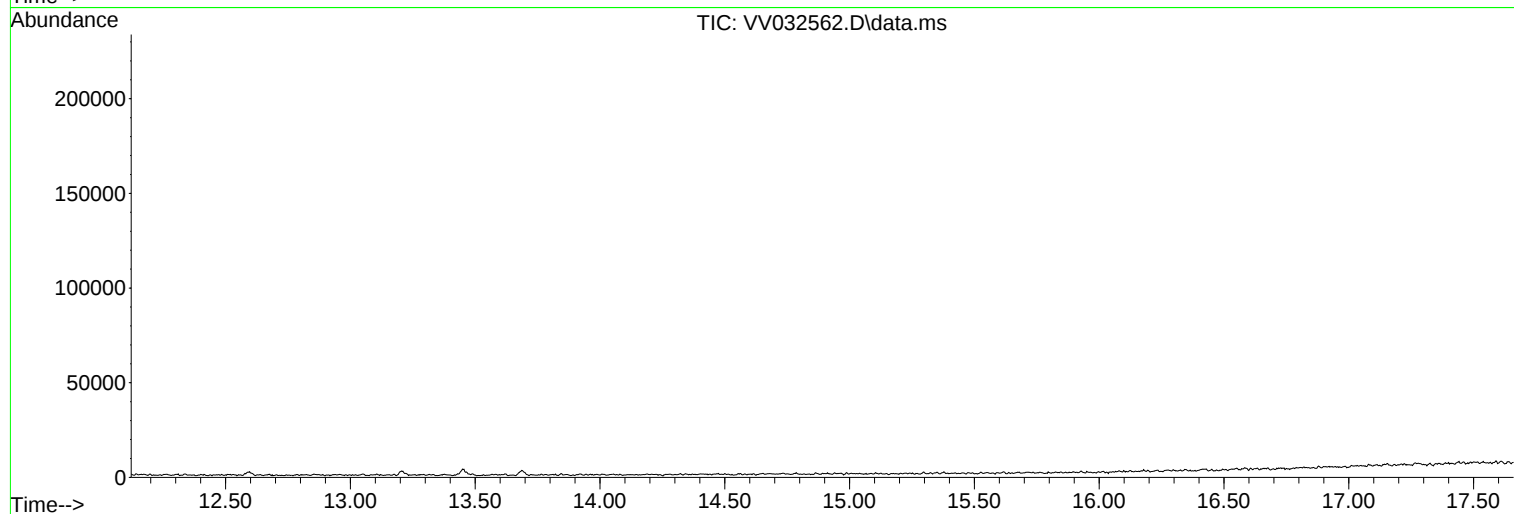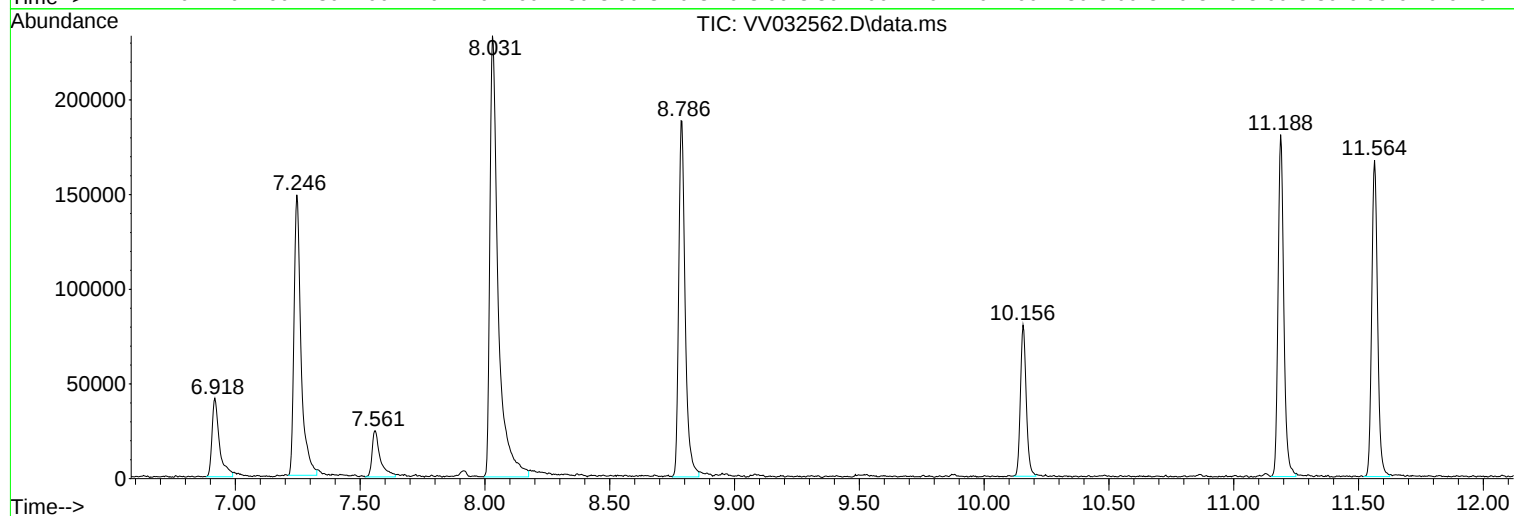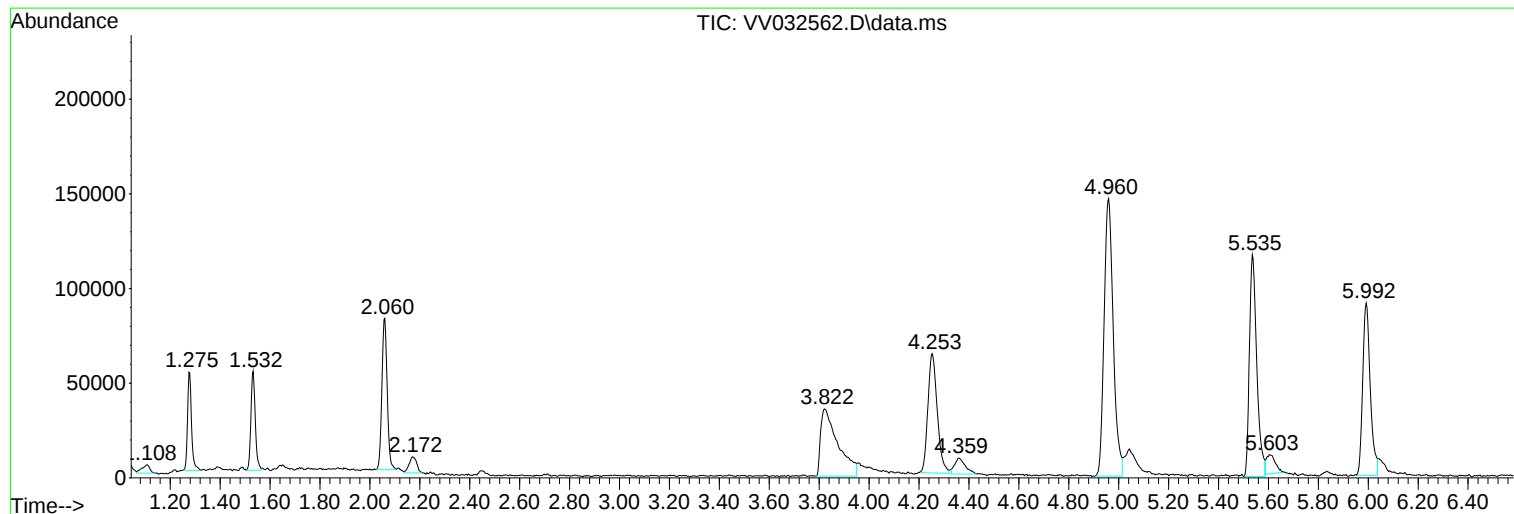

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032562.D
Acq On : 23 Oct 2023 11:43
Operator : SY/MD
Sample : VV1023WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK376

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032562.D
Acq On : 23 Oct 2023 11:43
Operator : SY/MD
Sample : VV1023WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK376

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc