

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
 Data File : VV032566.D
 Acq On : 23 Oct 2023 13:29
 Operator : SY/MD
 Sample : 04993-02DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032566.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	65	74	85	rBV	45959	53236	9.99%	1.317%
2	1.532	146	153	164	rBV	46497	54572	10.24%	1.350%
3	2.053	305	315	331	rVB	96971	141599	26.57%	3.502%
4	2.445	428	437	450	rBV3	6984	12365	2.32%	0.306%
5	2.558	462	472	481	rBV	5601	10206	1.92%	0.252%
6	3.825	853	866	898	rBV2	44564	215452	40.43%	5.328%
7	4.249	981	998	1022	rBV2	68669	184424	34.60%	4.561%
8	4.960	1201	1219	1240	rBV2	152241	391663	73.49%	9.686%
9	5.535	1385	1398	1423	rBV2	133316	285960	53.66%	7.072%
10	5.992	1527	1540	1562	rBV	93396	199876	37.50%	4.943%
11	6.918	1817	1828	1850	rBV	42334	85727	16.09%	2.120%
12	7.246	1919	1930	1953	rBV	154980	284073	53.30%	7.025%
13	7.561	2017	2028	2042	rBV2	26499	50458	9.47%	1.248%
14	7.905	2119	2135	2154	rBV	247650	433289	81.30%	10.716%
15	8.034	2163	2175	2214	rBV	241029	532948	100.00%	13.180%
16	8.786	2398	2409	2434	rBV	208472	361985	67.92%	8.952%
17	10.156	2825	2835	2852	rBV	80923	131315	24.64%	3.248%
18	11.188	3146	3156	3175	rBV	200269	319121	59.88%	7.892%
19	11.564	3262	3273	3288	rBV	166965	272240	51.08%	6.733%
20	12.587	3584	3591	3596	rBV6	4655	6697	1.26%	0.166%
21	13.207	3773	3784	3796	rBV6	6611	10482	1.97%	0.259%
22	13.686	3924	3933	3941	rBV7	4070	5864	1.10%	0.145%




Sum of corrected areas: 4043552

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032566.D
Acq On : 23 Oct 2023 13:29
Operator : SY/MD
Sample : 04993-02DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

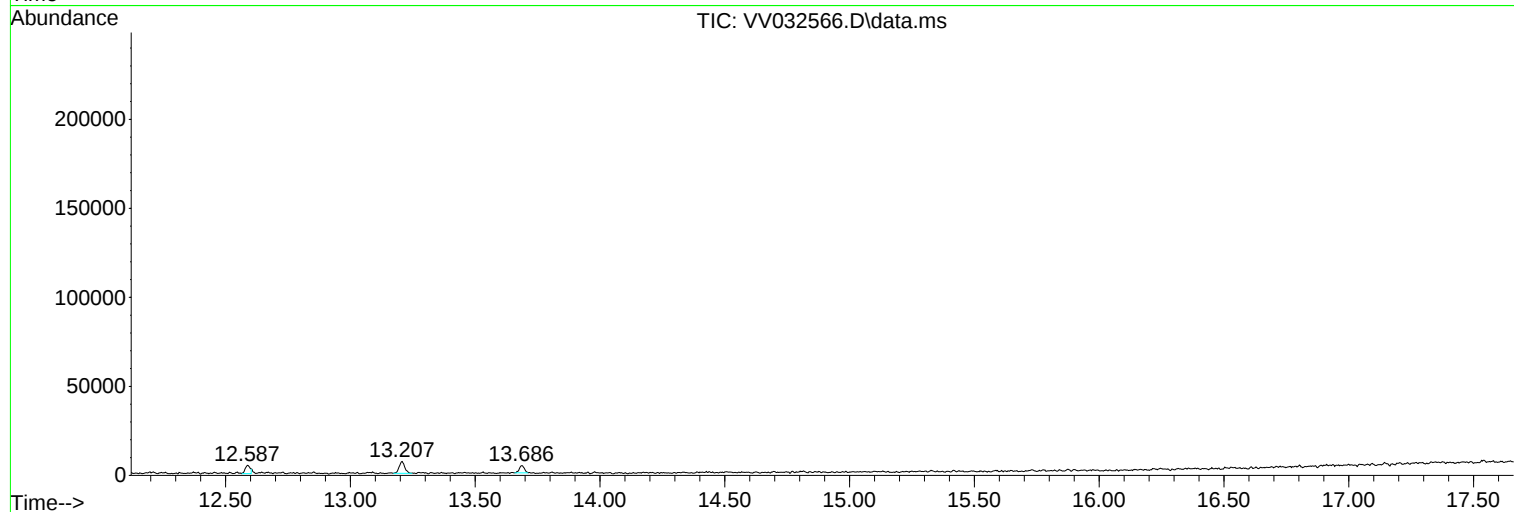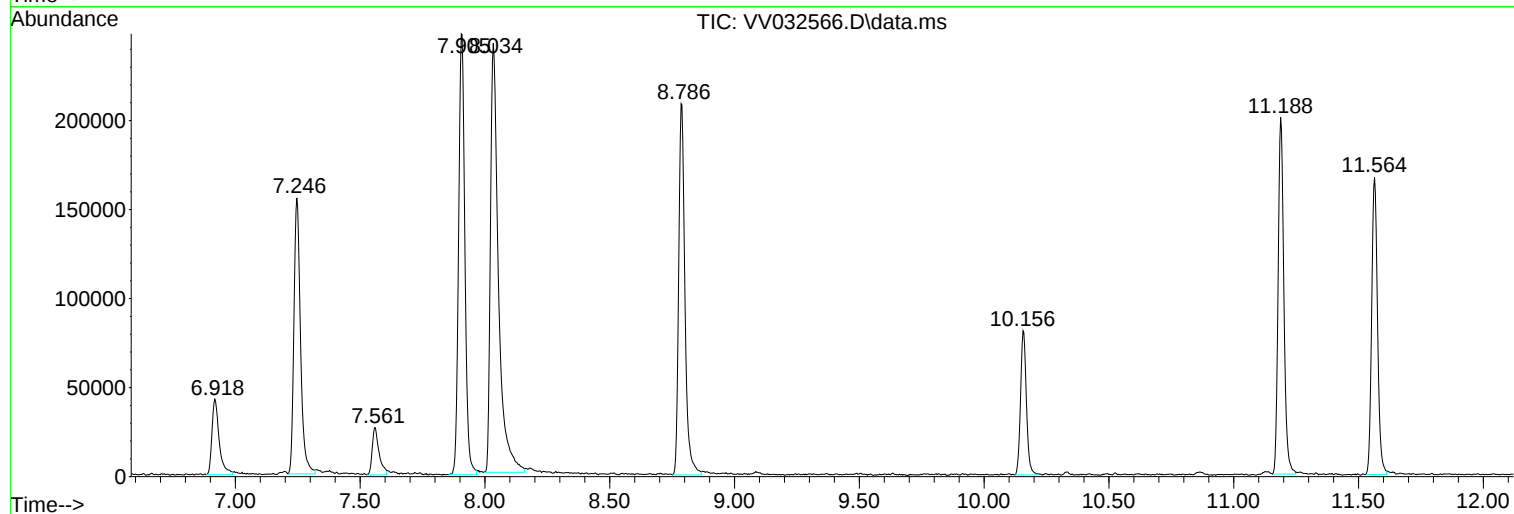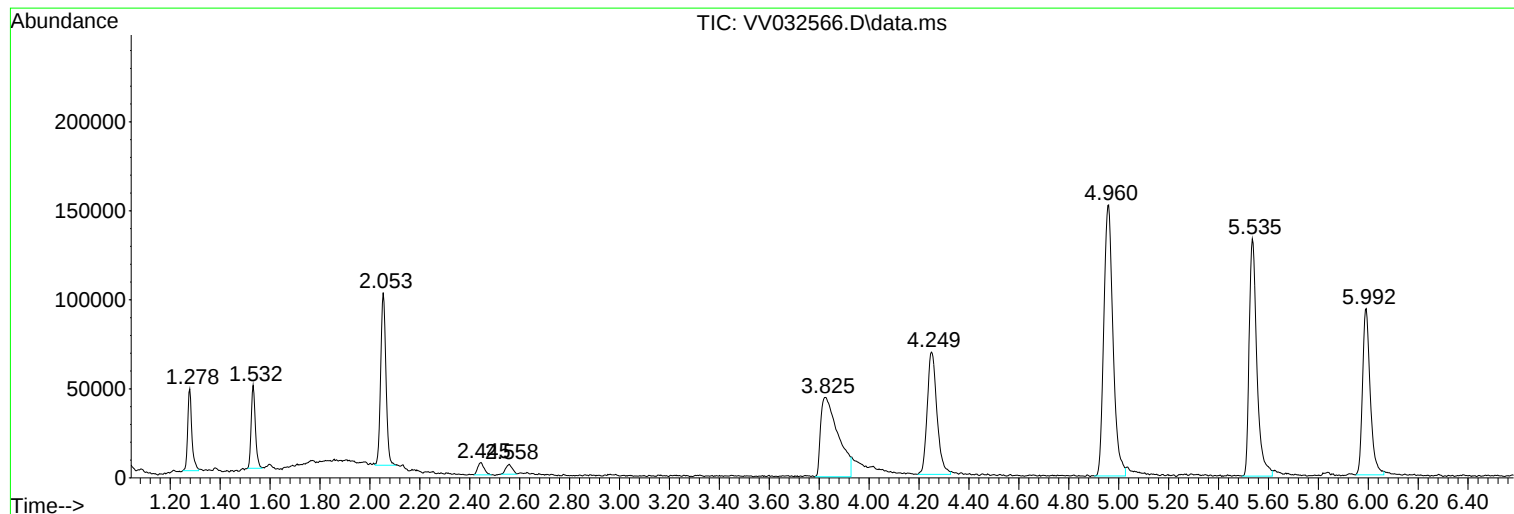

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032566.D
Acq On : 23 Oct 2023 13:29
Operator : SY/MD
Sample : 04993-02DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032566.D
Acq On : 23 Oct 2023 13:29
Operator : SY/MD
Sample : 04993-02DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc