

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
 Data File : VV032567.D
 Acq On : 23 Oct 2023 13:53
 Operator : SY/MD
 Sample : 04993-03DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032567.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rBV	48985	53211	9.08%	1.295%
2	1.532	144	153	169	rVB	51466	60948	10.40%	1.483%
3	2.060	308	317	328	rVB	79766	115313	19.68%	2.805%
4	2.175	345	353	363	rVB5	7169	13903	2.37%	0.338%
5	2.449	429	438	456	rVB3	7499	15218	2.60%	0.370%
6	3.825	852	866	905	rBV3	49326	242212	41.34%	5.893%
7	4.252	984	999	1022	rBV	63330	166030	28.34%	4.039%
8	4.359	1024	1032	1053	rVB4	6772	18615	3.18%	0.453%
9	4.960	1204	1219	1239	rBV2	144243	378842	64.66%	9.216%
10	5.539	1388	1399	1415	rBV	118191	251009	42.84%	6.107%
11	5.992	1522	1540	1571	rBV2	90447	210886	35.99%	5.130%
12	6.918	1816	1828	1848	rBV	40153	82209	14.03%	2.000%
13	7.246	1915	1930	1958	rBV	147057	287326	49.04%	6.990%
14	7.561	2018	2028	2046	rBV2	25283	49835	8.51%	1.212%
15	7.908	2123	2136	2164	rBV	323106	585916	100.00%	14.254%
16	8.030	2164	2174	2209	rBV	254635	535834	91.45%	13.036%
17	8.789	2397	2410	2431	rBV	194838	344721	58.83%	8.386%
18	10.156	2825	2835	2849	rBV	82244	131901	22.51%	3.209%
19	11.188	3146	3156	3172	rBV	184973	296516	50.61%	7.214%
20	11.564	3261	3273	3296	rBV	167365	270031	46.09%	6.569%




Sum of corrected areas: 4110476

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032567.D
Acq On : 23 Oct 2023 13:53
Operator : SY/MD
Sample : 04993-03DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

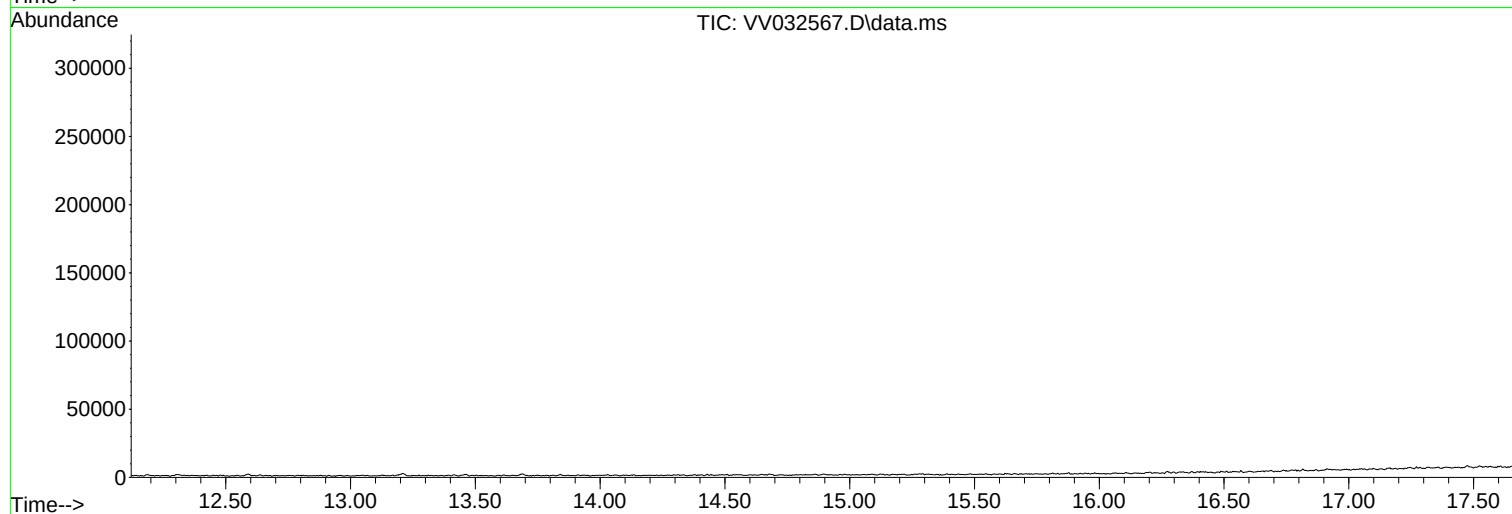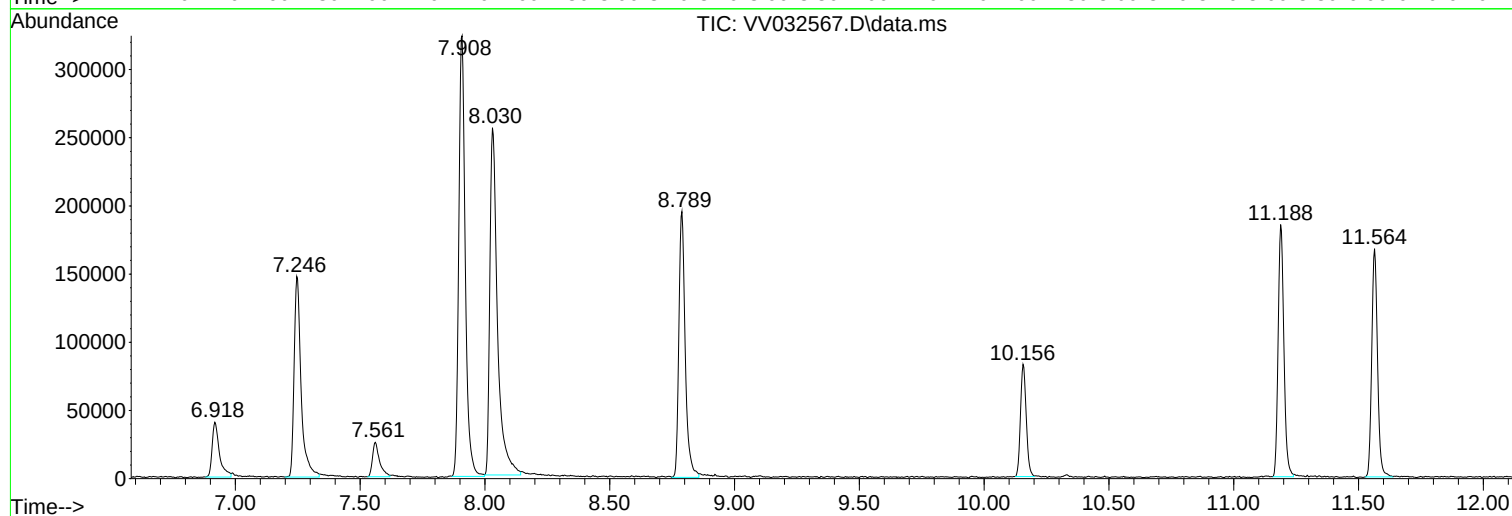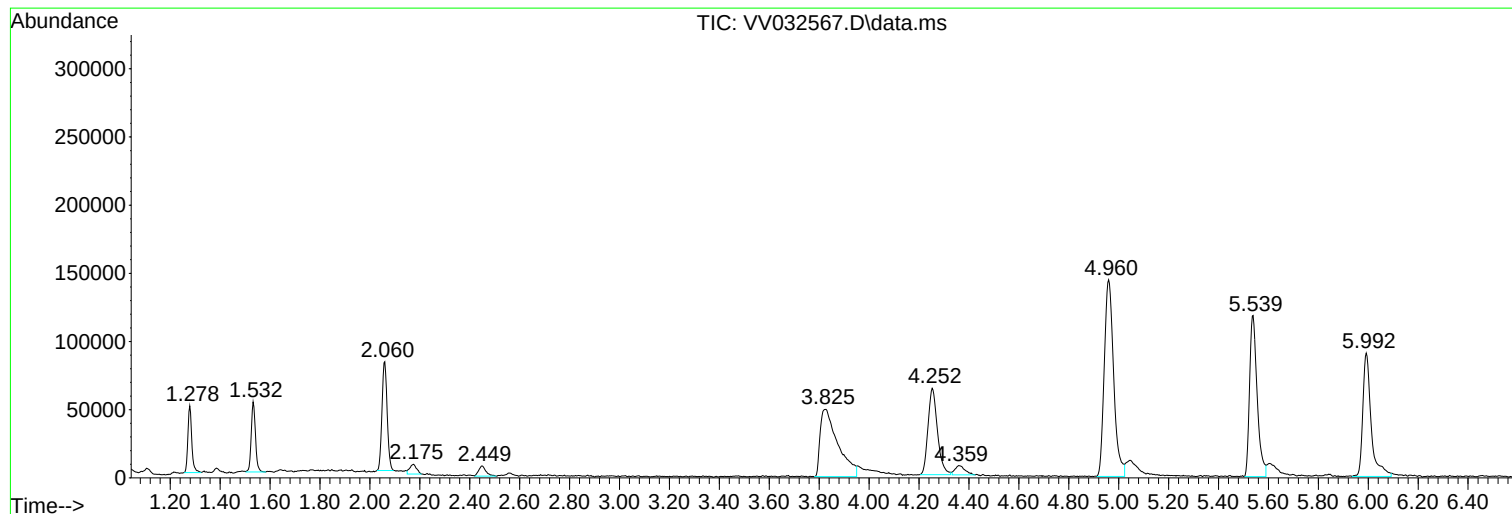

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032567.D
Acq On : 23 Oct 2023 13:53
Operator : SY/MD
Sample : 04993-03DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032567.D
Acq On : 23 Oct 2023 13:53
Operator : SY/MD
Sample : 04993-03DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc