

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
 Data File : VV032568.D
 Acq On : 23 Oct 2023 14:17
 Operator : SY/MD
 Sample : 04993-04DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032568.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	18	23	31	rVB	4164	5556	1.10%	0.146%
2	1.278	67	74	83	rBV	45739	48581	9.63%	1.280%
3	1.532	146	153	165	rVB	49203	57184	11.33%	1.506%
4	2.060	307	317	335	rBV	76683	113401	22.47%	2.987%
5	2.182	346	355	363	rVB2	6235	10732	2.13%	0.283%
6	2.449	429	438	450	rVB3	5726	10160	2.01%	0.268%
7	3.822	853	865	891	rBV2	41117	179009	35.47%	4.715%
8	4.252	980	999	1023	rBV	61924	162387	32.17%	4.277%
9	4.368	1025	1035	1050	rVB3	5960	15364	3.04%	0.405%
10	4.960	1204	1219	1237	rBV2	137361	351823	69.71%	9.267%
11	5.538	1388	1399	1415	rBV	115992	244932	48.53%	6.451%
12	5.992	1526	1540	1558	rBV	87270	189268	37.50%	4.985%
13	6.918	1818	1828	1849	rBV	37222	79286	15.71%	2.088%
14	7.246	1917	1930	1959	rBV	139203	273887	54.26%	7.214%
15	7.561	2018	2028	2042	rBV3	22682	45341	8.98%	1.194%
16	7.908	2120	2136	2163	rBV	261064	483215	95.74%	12.727%
17	8.034	2163	2175	2206	rBV	237019	504724	100.00%	13.294%
18	8.789	2397	2410	2432	rBV	195193	345756	68.50%	9.107%
19	10.156	2823	2835	2855	rBV	77232	127056	25.17%	3.347%
20	11.188	3145	3156	3173	rBV	186314	296331	58.71%	7.805%
21	11.564	3262	3273	3287	rBV	160571	252657	50.06%	6.655%




Sum of corrected areas: 3796650

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032568.D
Acq On : 23 Oct 2023 14:17
Operator : SY/MD
Sample : 04993-04DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

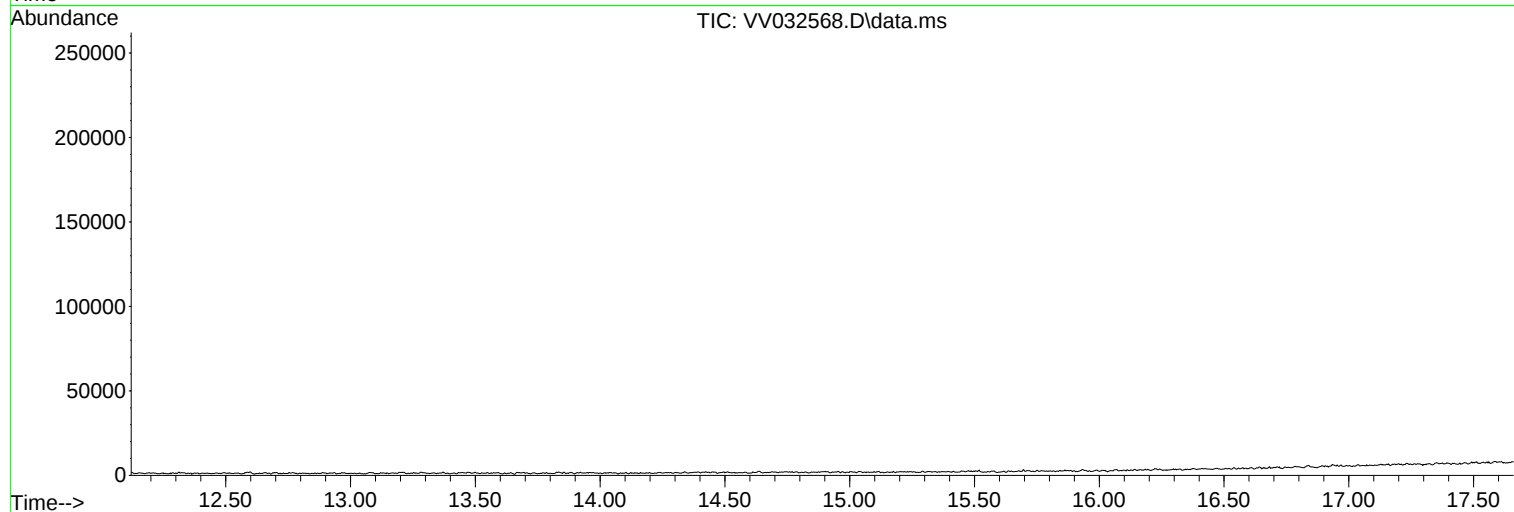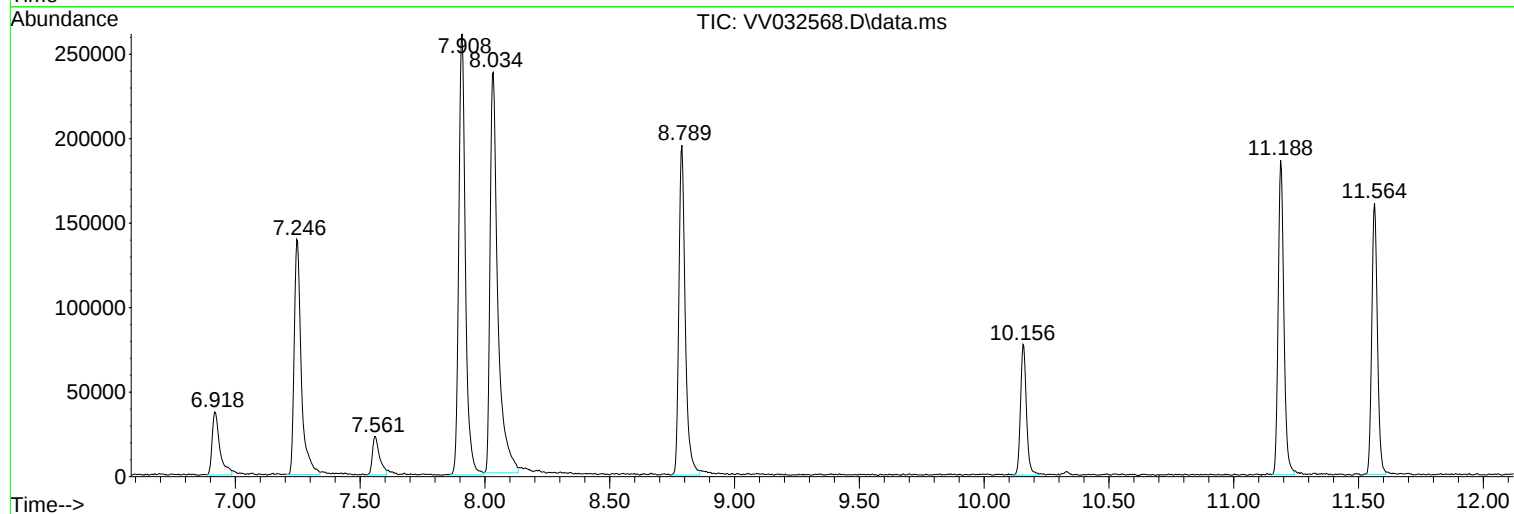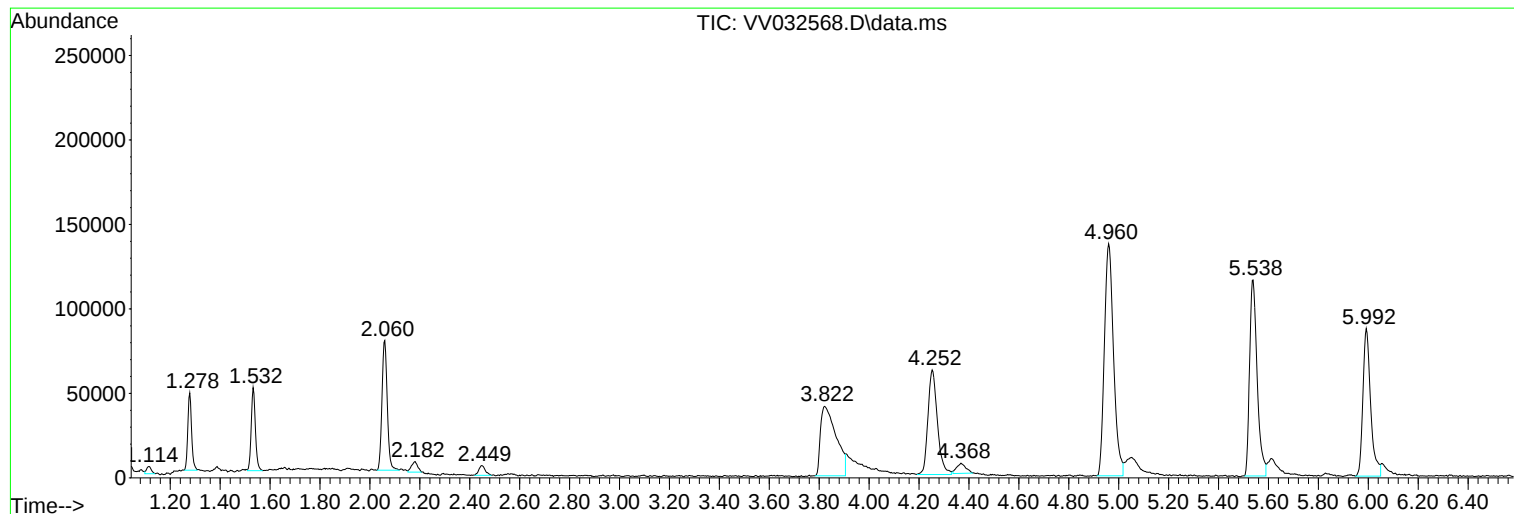

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032568.D
Acq On : 23 Oct 2023 14:17
Operator : SY/MD
Sample : 04993-04DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032568.D
Acq On : 23 Oct 2023 14:17
Operator : SY/MD
Sample : 04993-04DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc