

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
 Data File : VV032569.D
 Acq On : 23 Oct 2023 14:41
 Operator : SY/MD
 Sample : 04993-19DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B00DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032569.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	18	rBV2	3649	3703	1.02%	0.180%
2	1.114	18	23	31	rVB	4112	5736	1.57%	0.278%
3	1.278	65	74	82	rBV	23941	28471	7.81%	1.381%
4	1.532	146	153	161	rVB	23945	28693	7.87%	1.392%
5	2.060	308	317	328	rBV	34374	51570	14.14%	2.502%
6	2.449	432	438	453	rVB7	5528	10793	2.96%	0.524%
7	3.793	847	856	883	rBV2	55153	167823	46.03%	8.142%
8	4.256	984	1000	1021	rBV	28545	75906	20.82%	3.682%
9	4.371	1021	1036	1044	rBV6	3560	8819	2.42%	0.428%
10	4.960	1205	1219	1239	rBV4	65525	176437	48.39%	8.559%
11	5.539	1389	1399	1417	rBV	51097	112782	30.93%	5.471%
12	5.992	1529	1540	1556	rBV2	39978	87889	24.11%	4.264%
13	6.921	1819	1829	1845	rBV2	17121	36352	9.97%	1.764%
14	7.249	1920	1931	1957	rBV	58512	118309	32.45%	5.740%
15	7.564	2019	2029	2042	rBV2	11699	22967	6.30%	1.114%
16	7.908	2120	2136	2159	rBV	146102	266220	73.02%	12.915%
17	8.031	2164	2174	2208	rBV	174377	364598	100.00%	17.688%
18	8.789	2400	2410	2428	rBV	86925	156439	42.91%	7.589%
19	10.156	2822	2835	2850	rBV	50804	85137	23.35%	4.130%
20	11.191	3147	3157	3176	rBV	82258	134957	37.02%	6.547%
21	11.564	3263	3273	3286	rBV	72677	117707	32.28%	5.710%




Sum of corrected areas: 2061308

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032569.D
Acq On : 23 Oct 2023 14:41
Operator : SY/MD
Sample : 04993-19DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

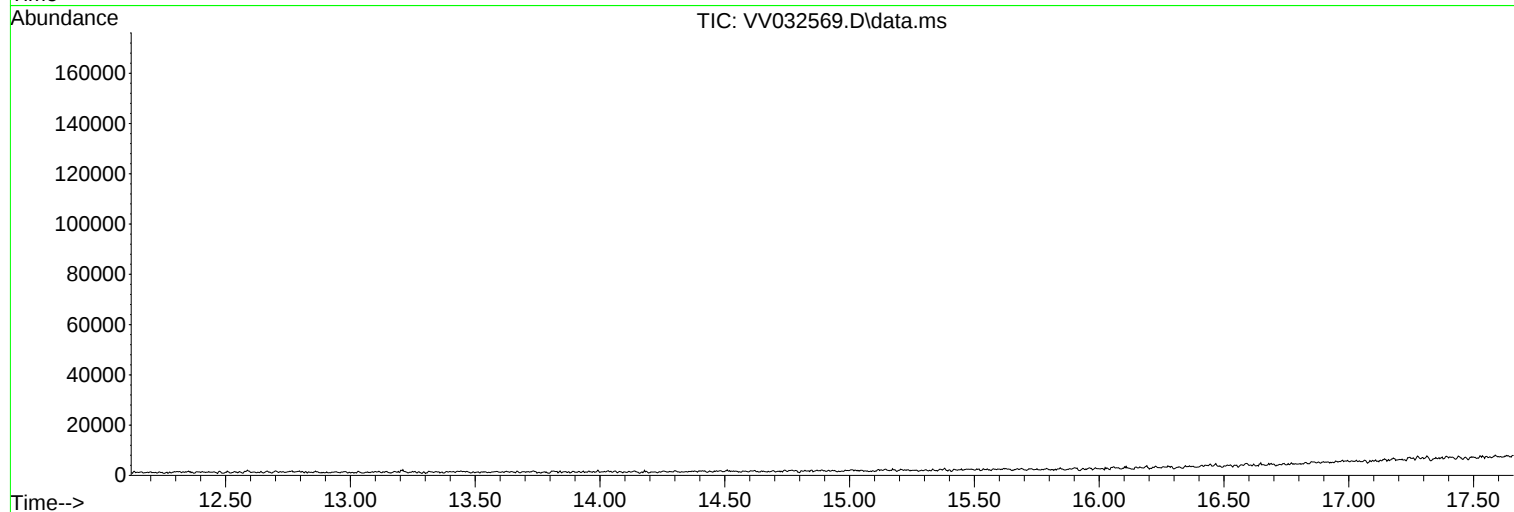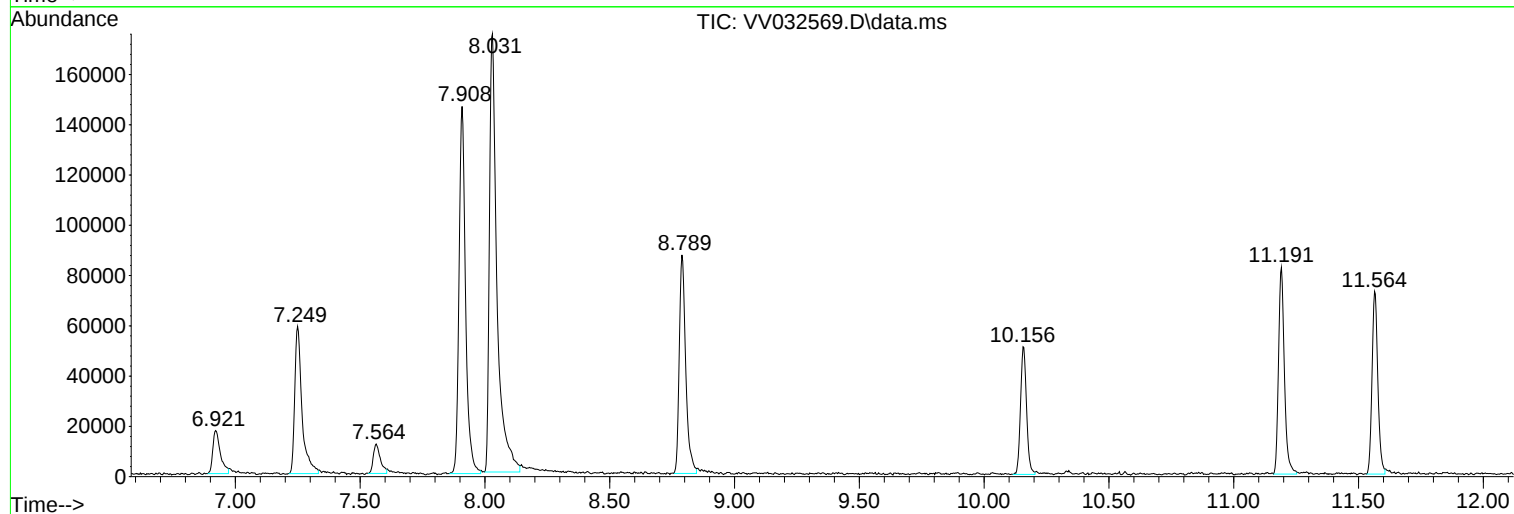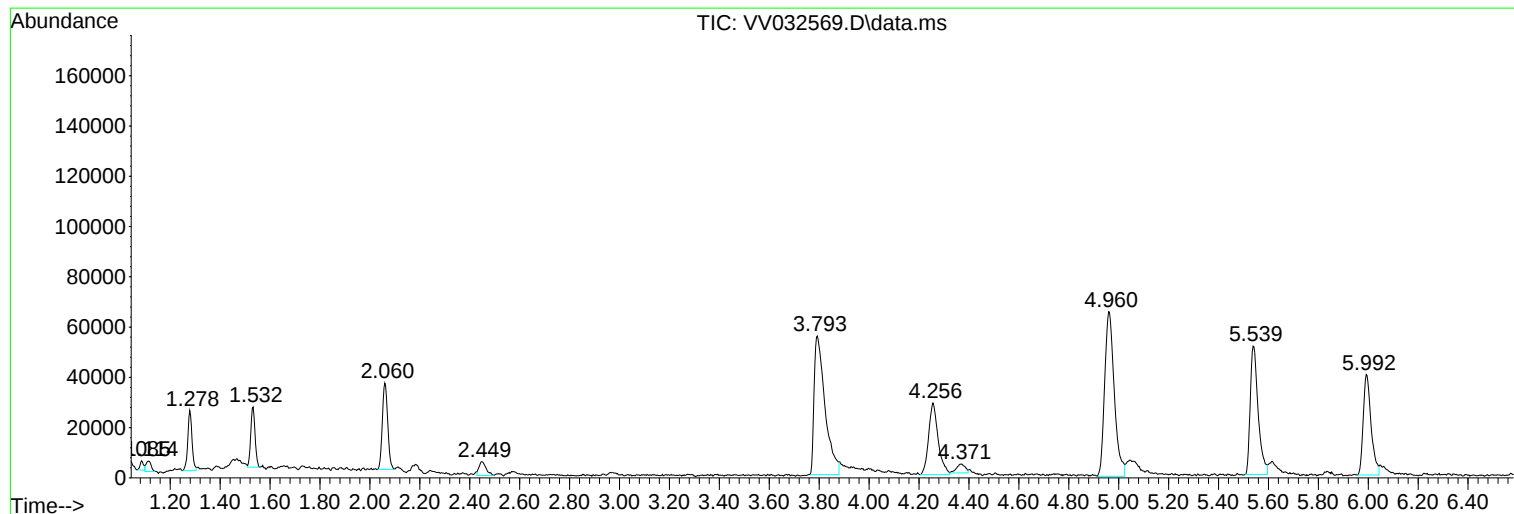

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032569.D
Acq On : 23 Oct 2023 14:41
Operator : SY/MD
Sample : 04993-19DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032569.D
Acq On : 23 Oct 2023 14:41
Operator : SY/MD
Sample : 04993-19DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B00DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc