

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
 Data File : VV032570.D
 Acq On : 23 Oct 2023 15:06
 Operator : SY/MD
 Sample : 04993-16DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AY7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	19	23	37	rVB	6036	9064	1.83%	0.255%
2	1.275	66	73	89	rVB	44530	49931	10.07%	1.406%
3	1.532	145	153	163	rBV	47815	55857	11.26%	1.573%
4	2.056	307	316	332	rVB	77313	112443	22.68%	3.167%
5	2.179	346	354	365	rVB5	7350	13566	2.74%	0.382%
6	2.445	428	437	452	rVB6	5571	11487	2.32%	0.324%
7	3.828	856	867	910	rBV2	35184	186557	37.62%	5.255%
8	4.252	982	999	1022	rBV	58398	154056	31.07%	4.339%
9	4.362	1024	1033	1034	rBV8	5219	5660	1.14%	0.159%
10	4.960	1199	1219	1238	rBV3	133808	348269	70.24%	9.809%
11	5.535	1384	1398	1417	rBV	115669	247587	49.93%	6.974%
12	5.992	1527	1540	1556	rBV	82600	177997	35.90%	5.013%
13	6.918	1818	1828	1857	rBV2	35906	77319	15.59%	2.178%
14	7.246	1919	1930	1962	rBV	133591	262026	52.84%	7.380%
15	7.561	2019	2028	2047	rBV2	22168	44631	9.00%	1.257%
16	7.908	2120	2136	2162	rBV	171174	315924	63.71%	8.898%
17	8.034	2162	2175	2211	rBV	225626	495850	100.00%	13.966%
18	8.789	2398	2410	2434	rBV	189214	330533	66.66%	9.310%
19	10.156	2825	2835	2850	rBV2	74303	121827	24.57%	3.431%
20	11.188	3146	3156	3177	rBV	176879	285141	57.51%	8.031%
21	11.564	3259	3273	3289	rBV	149509	244648	49.34%	6.891%




Sum of corrected areas: 3550373

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032570.D
Acq On : 23 Oct 2023 15:06
Operator : SY/MD
Sample : 04993-16DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AY7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

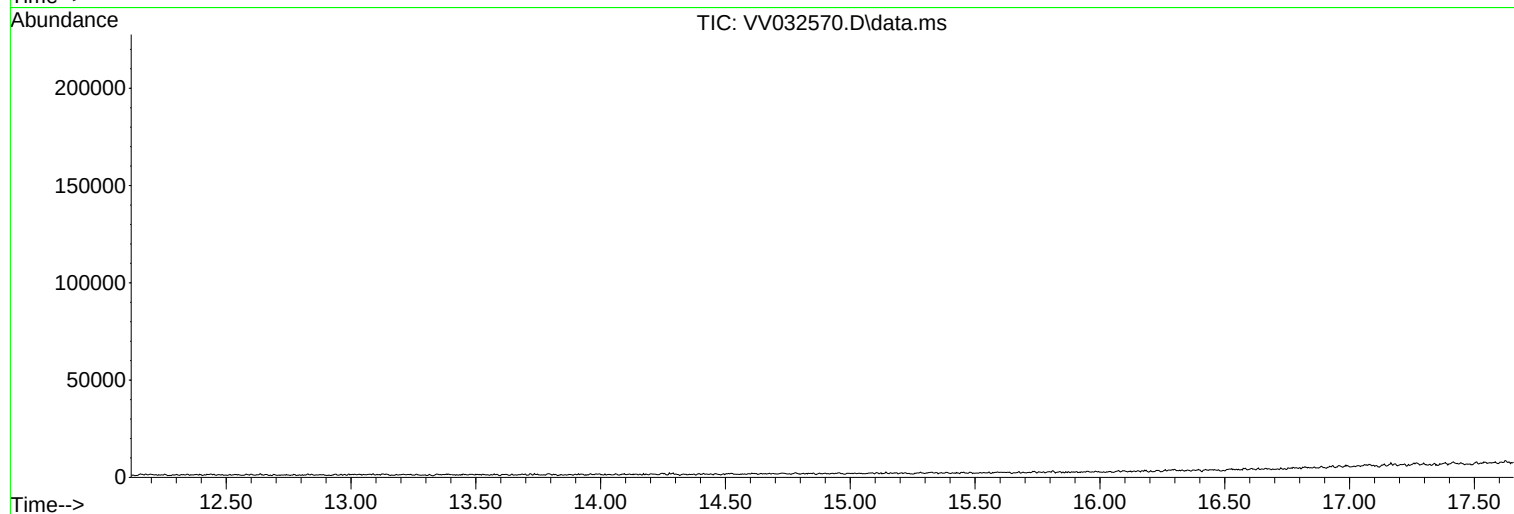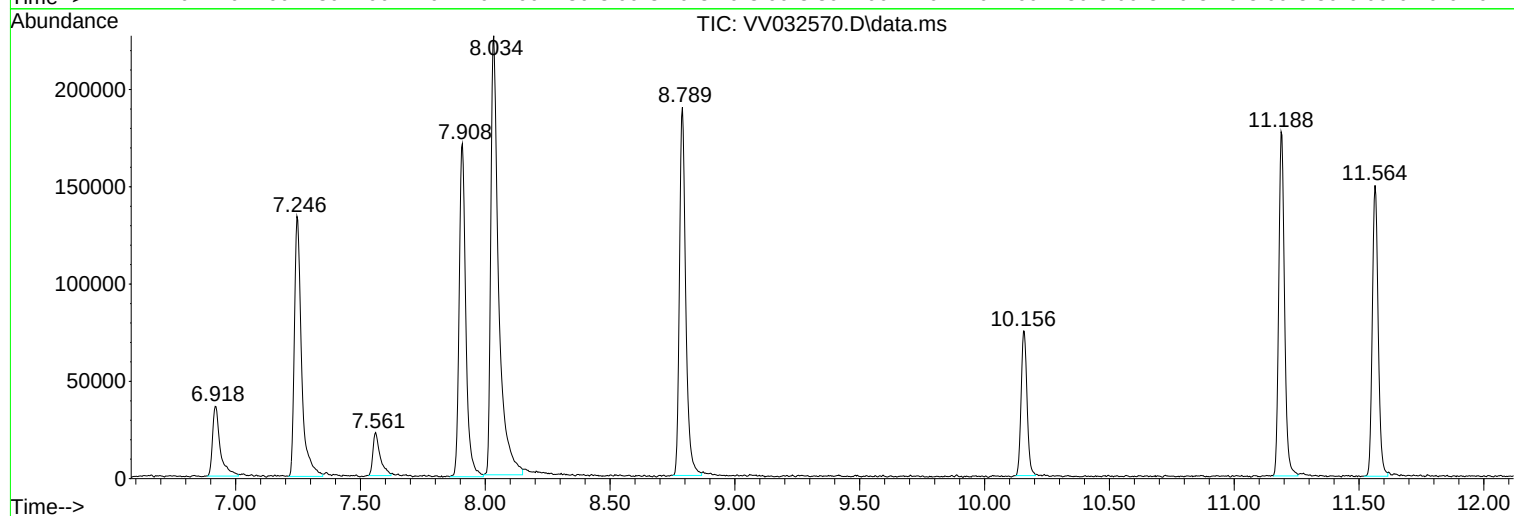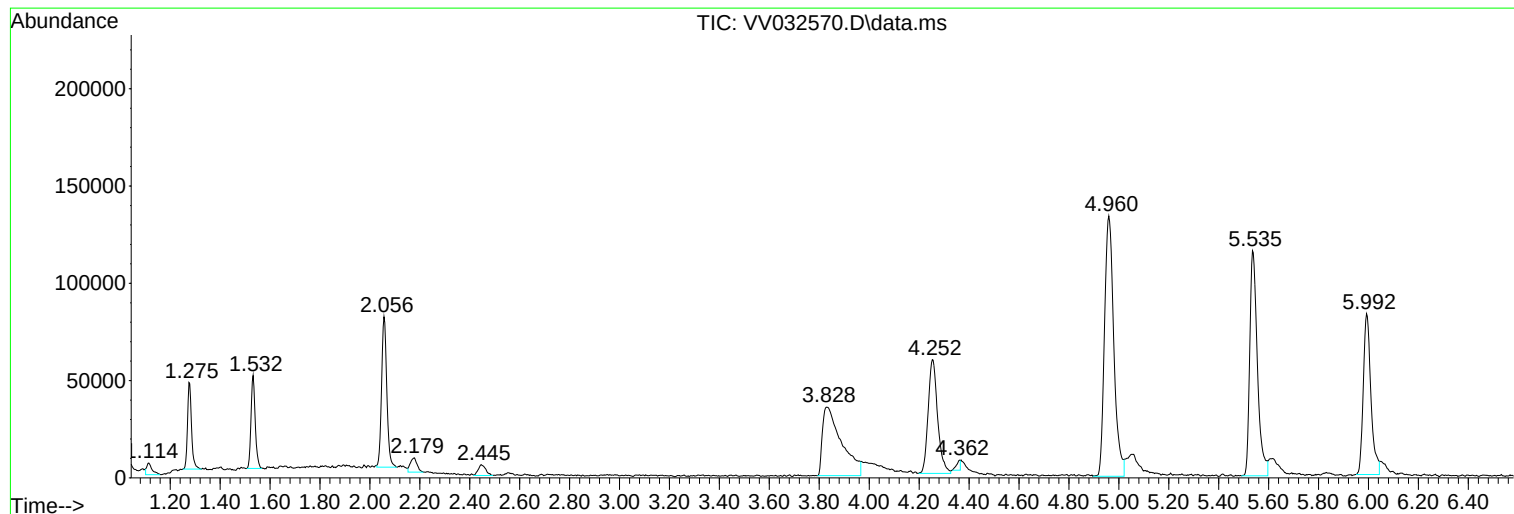

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032570.D
Acq On : 23 Oct 2023 15:06
Operator : SY/MD
Sample : 04993-16DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AY7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032570.D
Acq On : 23 Oct 2023 15:06
Operator : SY/MD
Sample : 04993-16DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AY7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------