

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
 Data File : VV032578.D
 Acq On : 23 Oct 2023 18:18
 Operator : SY/MD
 Sample : 04994-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B29

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	83	rVB	20020	22597	6.98%	1.090%
2	1.352	92	97	104	rBV	3449	4198	1.30%	0.203%
3	1.500	125	143	148	rBV	104823	132678	40.98%	6.401%
4	2.056	307	316	329	rBV	36399	55644	17.18%	2.685%
5	2.127	330	338	352	rVB2	8278	17713	5.47%	0.855%
6	2.272	367	383	390	rBV2	5212	14411	4.45%	0.695%
7	2.349	401	407	413	rBV2	4159	6682	2.06%	0.322%
8	2.445	428	437	449	rVB3	8633	16129	4.98%	0.778%
9	3.799	847	858	888	rBV3	41843	141386	43.67%	6.821%
10	4.272	983	1005	1028	rBV4	67557	231287	71.43%	11.158%
11	4.960	1200	1219	1241	rBV4	65527	176437	54.49%	8.512%
12	5.539	1387	1399	1416	rBV2	54245	118300	36.54%	5.707%
13	5.992	1525	1540	1566	rBV3	41705	96626	29.84%	4.662%
14	6.439	1667	1679	1698	rBV	18140	38981	12.04%	1.881%
15	6.921	1819	1829	1844	rBV2	16632	34926	10.79%	1.685%
16	7.249	1920	1931	1949	rBV	57538	108337	33.46%	5.227%
17	7.564	2017	2029	2042	rBV2	11563	23571	7.28%	1.137%
18	7.911	2131	2137	2146	rVB6	3594	6408	1.98%	0.309%
19	8.030	2163	2174	2210	rBV	154186	323797	100.00%	15.622%
20	8.181	2215	2221	2231	rVB5	4665	8265	2.55%	0.399%
21	8.789	2397	2410	2426	rBV	90575	156784	48.42%	7.564%
22	10.156	2822	2835	2850	rBV2	46283	77961	24.08%	3.761%
23	10.323	2882	2887	2895	rBV5	2947	4045	1.25%	0.195%
24	11.188	3147	3156	3175	rBV	81670	135411	41.82%	6.533%
25	11.564	3263	3273	3288	rBV	68370	110830	34.23%	5.347%
26	12.294	3492	3500	3511	rBV9	5265	9346	2.89%	0.451%




Sum of corrected areas: 2072750

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032578.D
Acq On : 23 Oct 2023 18:18
Operator : SY/MD
Sample : 04994-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

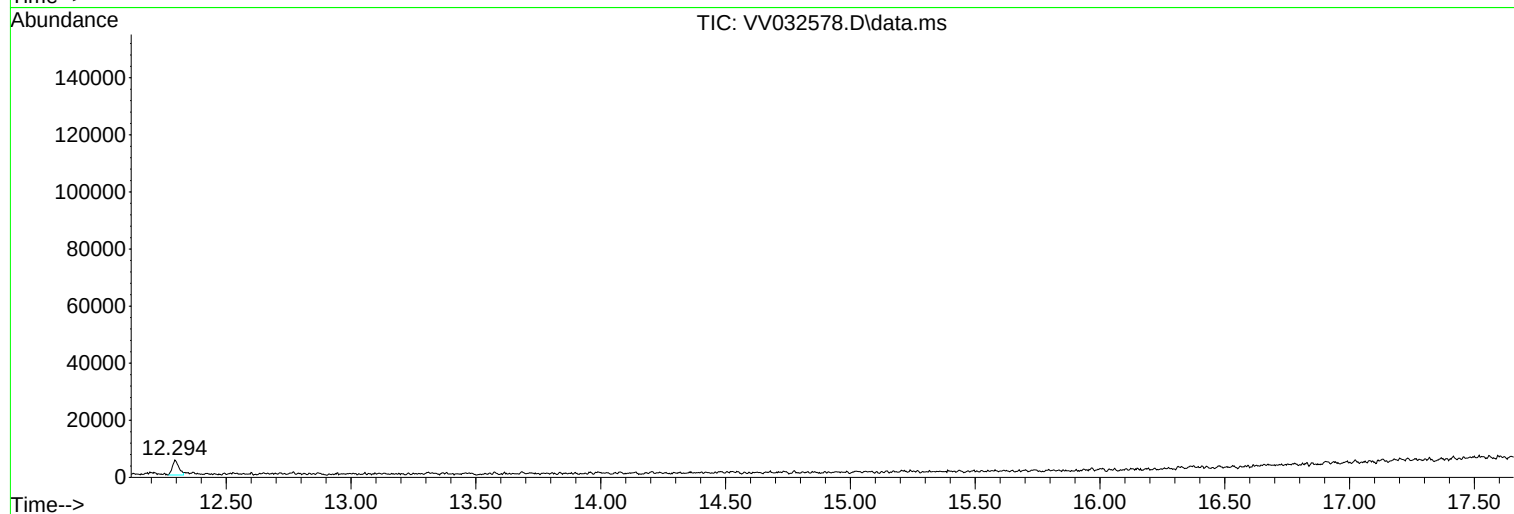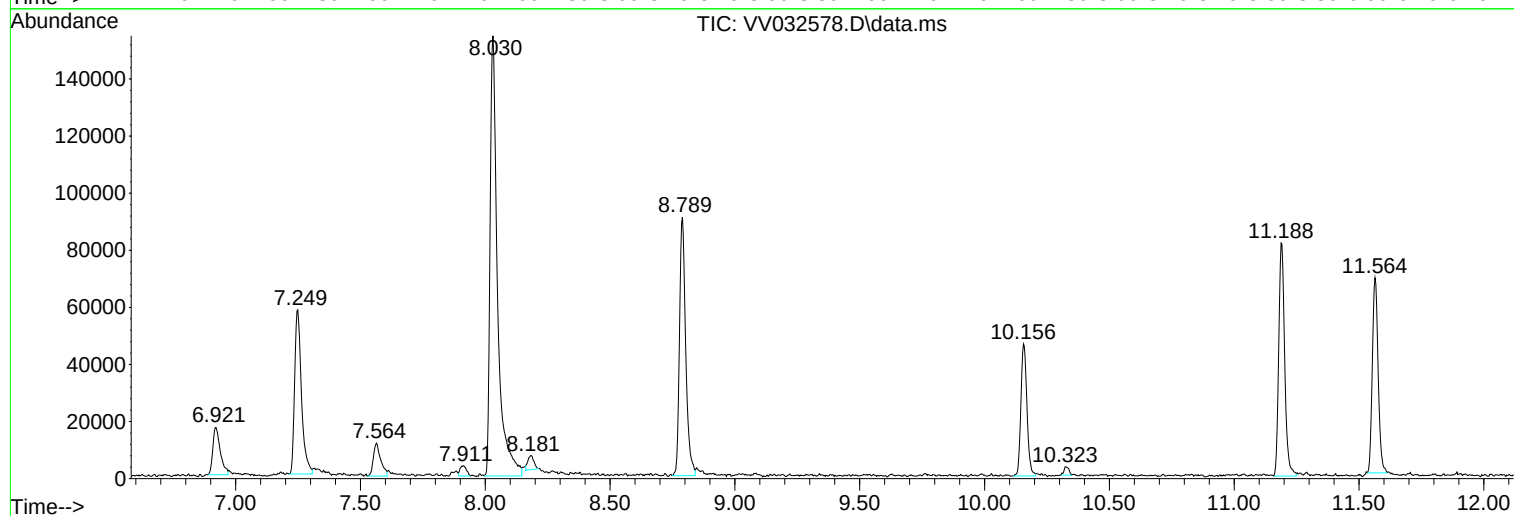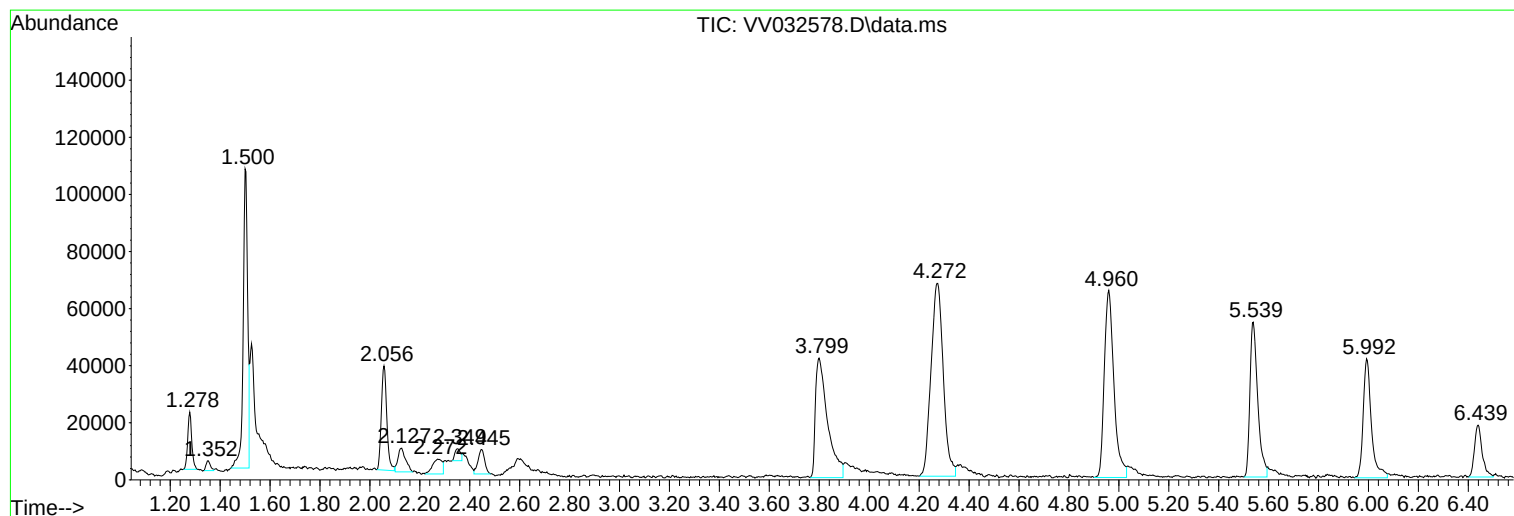

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032578.D
Acq On : 23 Oct 2023 18:18
Operator : SY/MD
Sample : 04994-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032578.D
Acq On : 23 Oct 2023 18:18
Operator : SY/MD
Sample : 04994-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc