

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
 Data File : VV032580.D
 Acq On : 23 Oct 2023 19:06
 Operator : SY/MD
 Sample : 04994-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B37

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032580.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	84	rBV	37121	40887	8.69%	1.245%
2	1.532	146	153	169	rVB	40542	48435	10.30%	1.475%
3	2.060	307	317	331	rBV	57192	85239	18.12%	2.595%
4	2.182	349	355	367	rVB3	9215	15083	3.21%	0.459%
5	3.831	853	868	901	rBV2	31529	158496	33.69%	4.826%
6	4.275	980	1006	1025	rBV4	114439	382470	81.30%	11.645%
7	4.391	1027	1042	1067	rVB5	25045	87666	18.63%	2.669%
8	4.960	1203	1219	1238	rBV2	111551	289135	61.46%	8.804%
9	5.539	1386	1399	1414	rBV	99704	211013	44.85%	6.425%
10	5.992	1526	1540	1556	rBV	73013	156469	33.26%	4.764%
11	6.439	1666	1679	1693	rBV2	31582	67247	14.29%	2.048%
12	6.918	1818	1828	1858	rBV	29893	66508	14.14%	2.025%
13	7.246	1918	1930	1951	rBV	106583	218035	46.34%	6.639%
14	7.561	2017	2028	2046	rBV2	19023	39912	8.48%	1.215%
15	8.034	2164	2175	2212	rBV	208168	470465	100.00%	14.325%
16	8.182	2213	2221	2235	rVB4	8567	19381	4.12%	0.590%
17	8.789	2397	2410	2439	rBV	171369	313441	66.62%	9.544%
18	10.156	2824	2835	2851	rBV	70092	116705	24.81%	3.553%
19	11.188	3145	3156	3175	rBV	165535	264544	56.23%	8.055%
20	11.564	3259	3273	3289	rBV	133134	217798	46.29%	6.631%
21	12.294	3490	3500	3510	rBV8	8276	15386	3.27%	0.468%




Sum of corrected areas: 3284315

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032580.D
Acq On : 23 Oct 2023 19:06
Operator : SY/MD
Sample : 04994-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

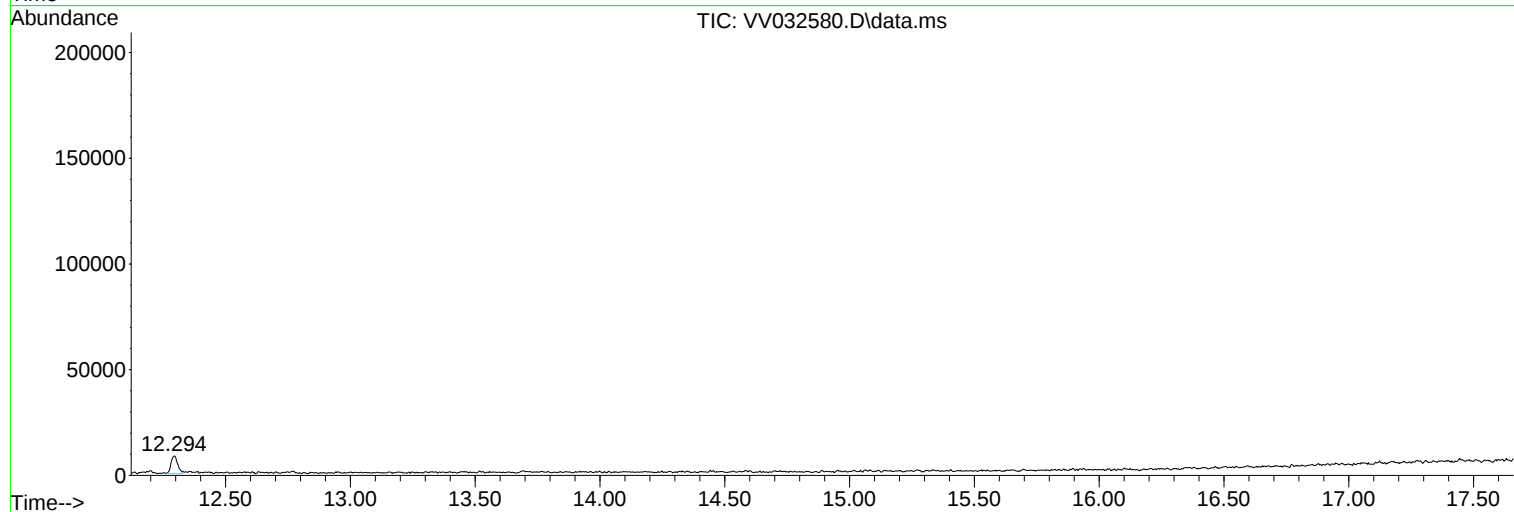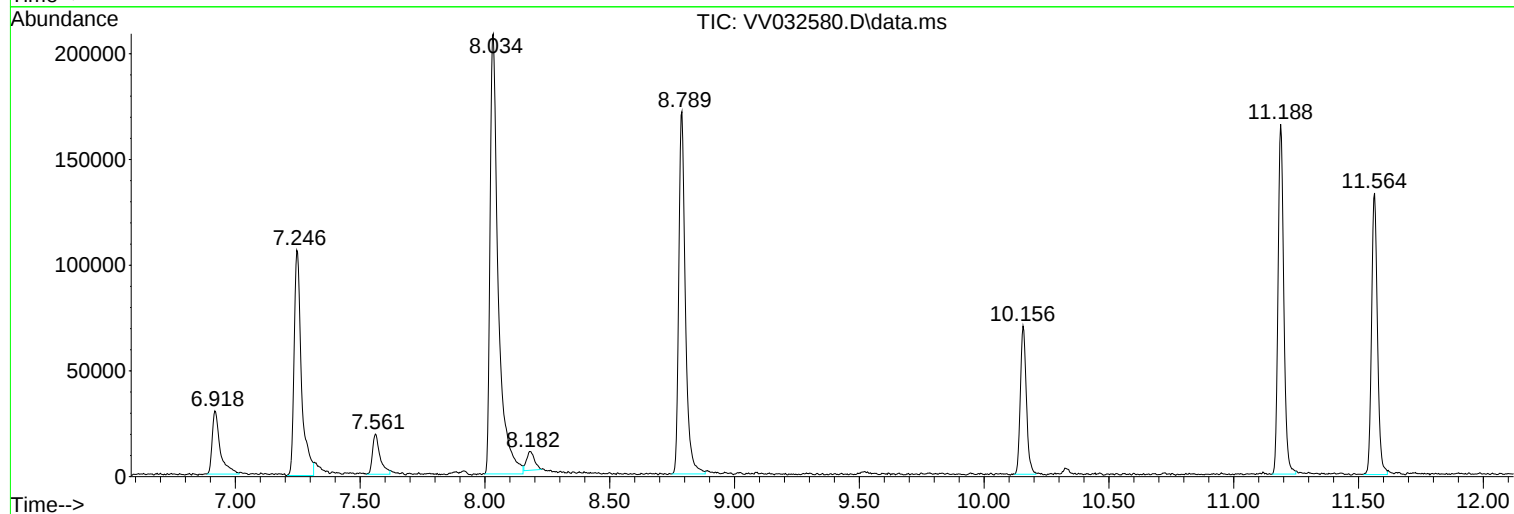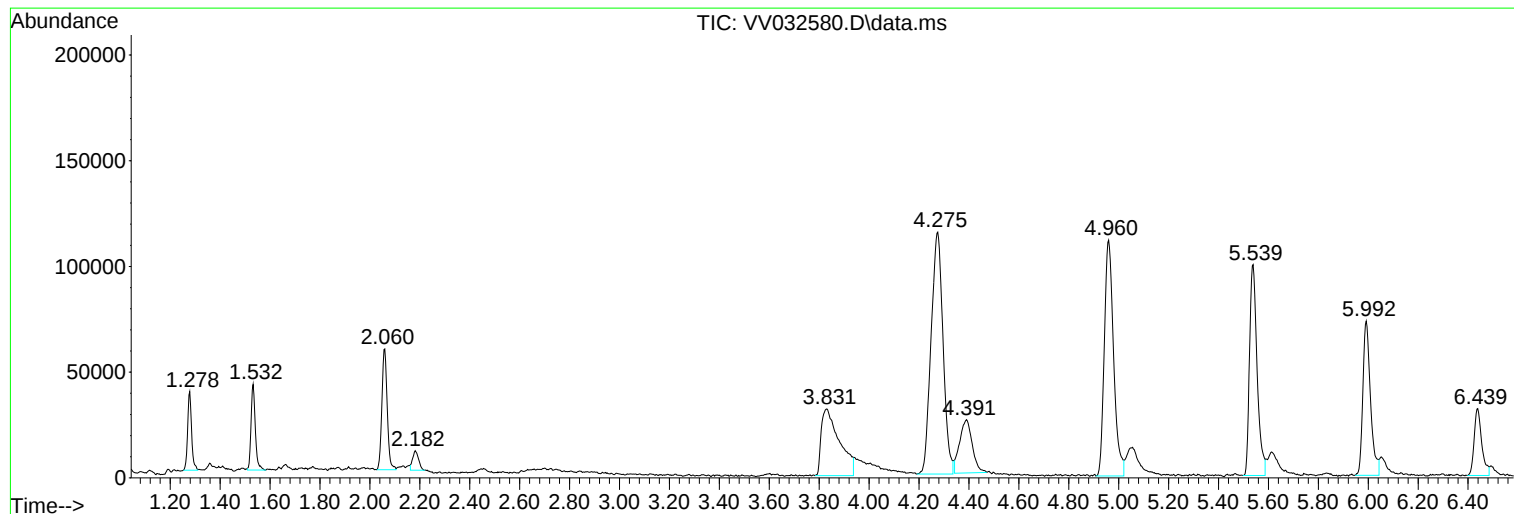

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032580.D
Acq On : 23 Oct 2023 19:06
Operator : SY/MD
Sample : 04994-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032580.D
Acq On : 23 Oct 2023 19:06
Operator : SY/MD
Sample : 04994-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc