
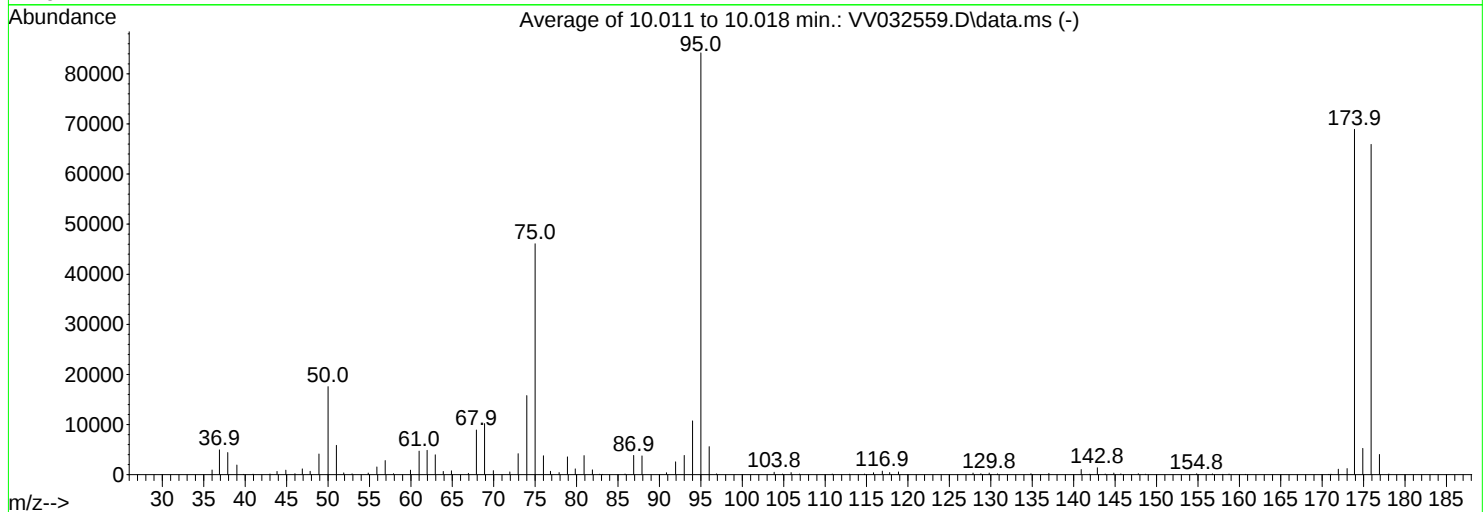


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102323\
Data File : VV032559.D
Acq On : 23 Oct 2023 08:39
Operator : SY/MD
Sample : BFB225
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB225

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Oct 26 04:59:52 2023

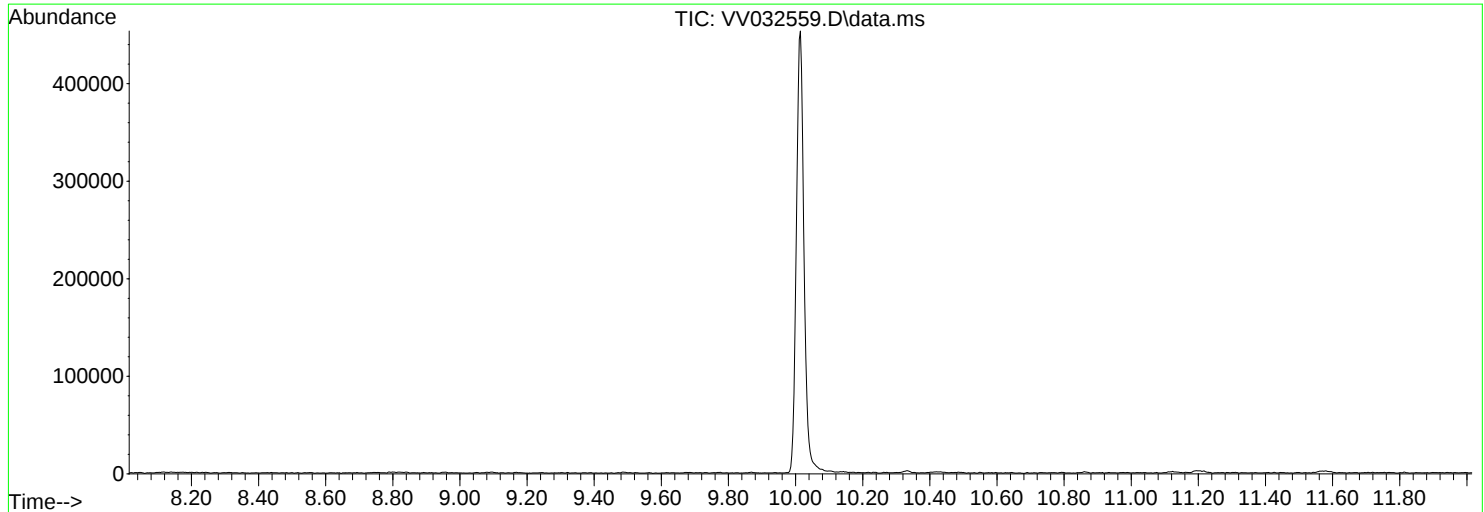

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	17579	PASS
75	95	30	80	54.7	46080	PASS
95	95	100	100	100.0	84195	PASS
96	95	5	9	6.6	5583	PASS
173	174	0.00	2	1.8	1229	PASS
174	95	50	120	81.8	68912	PASS
175	174	5	9	7.6	5246	PASS
176	174	95	105	95.7	65928	PASS
177	176	5	10	6.1	4018	PASS

m/z	Abundance
36.10	115.0
36.80	110.0
37.90	142.0
39.70	184.0
41.80	103.0
43.80	320.0
61.20	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
36.00	1088.0
36.90	5145.0
37.90	4863.0
39.00	1969.0
39.90	229.0
41.00	101.0
43.00	102.0
43.90	966.0
44.90	912.0
46.00	232.0
46.90	1227.0
47.90	755.0
48.90	4149.0
50.00	18352.0
51.00	6070.0
51.90	362.0
52.90	130.0
54.90	330.0
55.90	1588.0
56.90	2963.0
57.90	152.0
60.00	887.0
61.00	5005.0
62.00	5131.0
62.90	4085.0
63.90	665.0
64.90	741.0
66.90	283.0
67.90	9279.0
68.90	10540.0
70.00	861.0
72.00	574.0
72.90	4268.0
74.00	16296.0
75.00	47800.0
76.00	4006.0
76.80	666.0
77.90	436.0
78.90	3640.0
79.80	1144.0
80.90	3987.0
81.90	931.0
82.80	149.0
85.90	127.0
86.90	3778.0
87.90	3784.0
90.80	394.0
92.00	2569.0
93.00	3805.0
94.00	10901.0
95.00	85576.0
96.00	5866.0
96.90	178.0
103.90	501.0
104.80	145.0
105.90	472.0
106.90	124.0
110.80	135.0
113.00	102.0
114.80	153.0
115.80	416.0
116.90	748.0
117.80	429.0
118.90	539.0
127.80	375.0
128.80	179.0
129.80	287.0
130.80	147.0
134.90	211.0
137.00	251.0
140.90	1042.0
141.90	153.0
142.90	1349.0
143.80	123.0
144.90	387.0
145.70	166.0
147.80	187.0
148.70	150.0
150.00	104.0
154.90	200.0
156.70	130.0
158.70	116.0
160.70	106.0
170.80	174.0
171.90	1044.0
173.00	1293.0
173.90	69144.0
174.90	5307.0
175.90	64768.0
176.90	4051.0
178.00	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
36.00	1069.0
36.90	5251.0
38.00	4716.0
39.00	1987.0
39.90	241.0
40.90	105.0
41.80	136.0
43.00	137.0
43.90	988.0
44.90	924.0
46.00	210.0
46.90	1202.0
47.90	674.0
48.90	4285.0
50.00	18152.0
51.00	6076.0
51.90	338.0
52.90	149.0
54.80	343.0
55.90	1576.0
56.90	2903.0
57.90	205.0
59.90	922.0
61.00	5039.0
62.00	5000.0
63.00	4179.0
63.90	673.0
64.90	807.0
67.00	260.0
67.90	9175.0
68.90	10606.0
69.90	800.0
71.90	550.0
73.00	4321.0
74.00	16289.0
75.00	47888.0
76.00	3870.0
76.90	683.0
77.90	457.0
78.90	3647.0
79.90	1194.0
80.90	3916.0
81.90	989.0
82.80	134.0
85.90	145.0
86.90	4032.0
87.90	3906.0
90.90	396.0
91.90	2578.0
93.00	3981.0
94.00	11206.0
95.00	87312.0
96.00	5827.0
96.90	165.0
103.80	504.0
104.90	145.0
105.90	431.0
106.90	123.0
110.80	129.0
112.90	112.0
114.70	139.0
115.90	410.0
116.90	727.0
117.80	452.0
118.80	552.0
127.90	332.0
128.80	203.0
129.80	353.0
130.80	141.0
134.90	213.0
137.00	276.0
140.90	1044.0
142.90	1452.0
143.80	112.0
144.90	334.0
145.70	181.0
147.80	210.0
148.70	113.0
154.90	185.0
156.80	156.0
158.00	114.0
158.80	135.0
160.80	103.0
171.00	138.0
172.00	1130.0
173.00	1308.0
173.90	71272.0
174.90	5423.0
175.90	68472.0
176.90	4141.0
178.00	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
36.00	985.0
37.00	4768.0
38.00	4081.0
39.00	1828.0
39.90	249.0
40.90	105.0
41.80	158.0
43.00	162.0
43.90	933.0
44.90	807.0
46.00	188.0
46.90	1066.0
47.80	567.0
48.90	3983.0
50.00	16233.0
51.00	5384.0
51.90	337.0
52.90	173.0
54.90	298.0
55.90	1456.0
56.90	2521.0
57.90	232.0
59.90	880.0
61.00	4382.0
61.90	4402.0
63.00	3665.0
63.90	587.0
64.90	760.0
66.90	239.0
67.90	8255.0
68.90	9450.0
69.90	724.0
71.90	526.0
73.00	3956.0
74.00	14714.0
75.00	42552.0
76.00	3420.0
76.90	641.0
77.90	396.0
78.90	3327.0
79.90	1126.0
80.90	3480.0
81.90	934.0
83.10	158.0
85.80	168.0
86.90	3696.0
87.90	3566.0
90.90	409.0
91.90	2506.0
93.00	3750.0
94.00	10053.0
95.00	79696.0
96.00	5056.0
96.90	148.0
103.80	463.0
104.90	136.0
105.90	393.0
106.90	108.0
110.90	116.0
112.90	111.0
114.70	126.0
115.90	349.0
116.90	627.0
117.80	412.0
118.80	560.0
127.80	257.0
128.80	185.0
129.80	375.0
130.80	160.0
134.80	185.0
137.00	221.0
140.90	984.0
142.00	159.0
142.80	1334.0
143.80	112.0
144.80	261.0
145.70	153.0
147.80	182.0
154.80	181.0
156.80	186.0
158.00	126.0
158.80	144.0
171.10	119.0
172.00	1109.0
173.00	1085.0
173.90	66320.0
174.90	5009.0
175.90	64544.0
176.90	3863.0
178.10	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225