


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102418\
Data File : VV008387.D
Acq On : 24 Oct 2018 12:18
Operator : SY/MD
Sample : BFB49
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB49

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
Title : VOC Analysis
Last Update : Thu Oct 25 12:00:30 2018

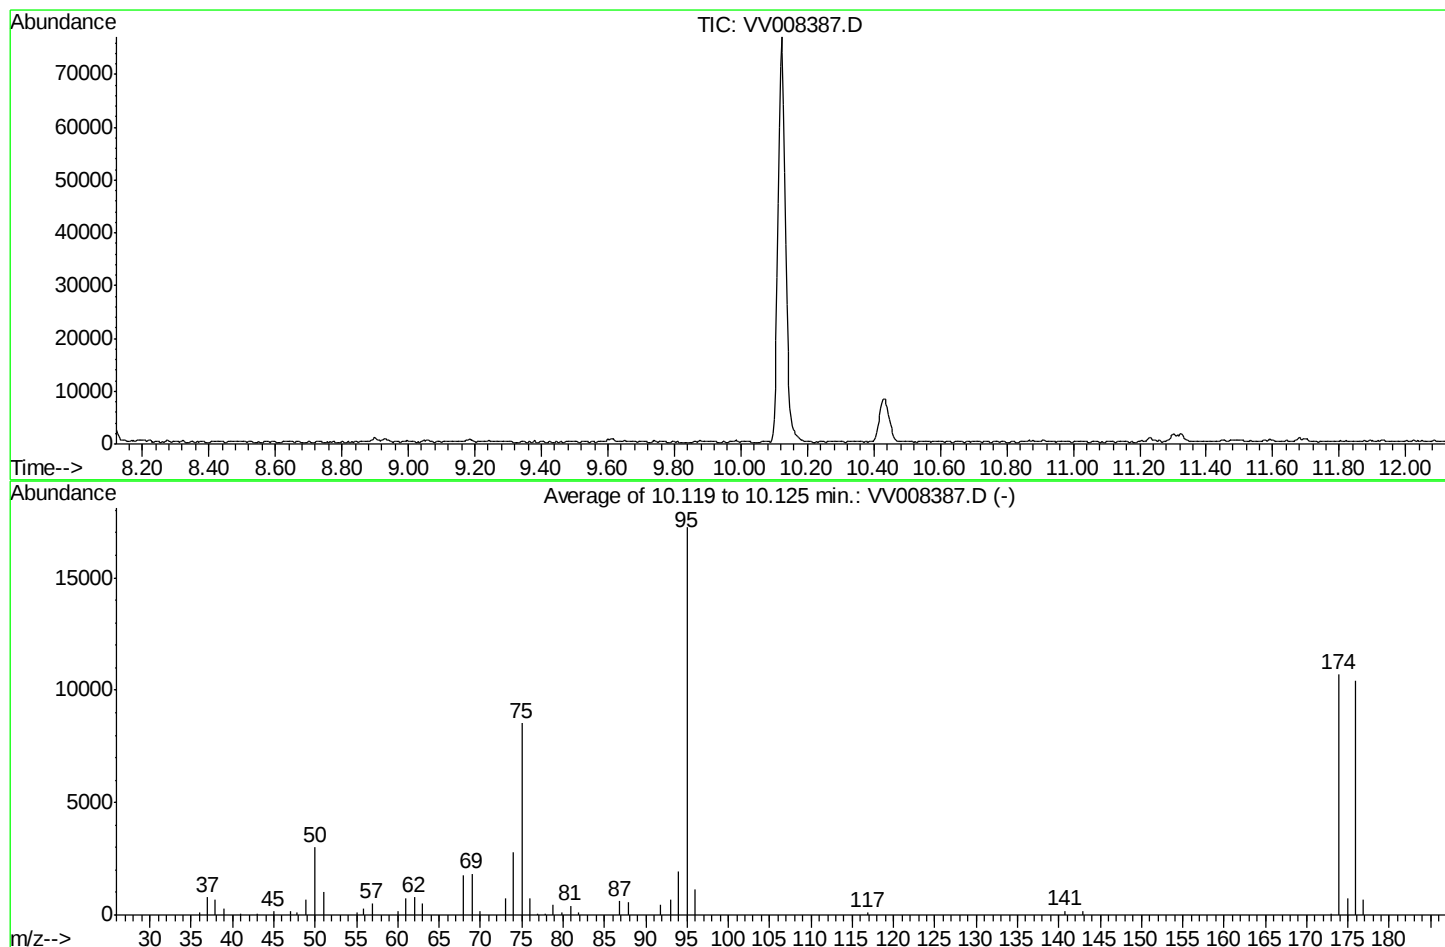

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	3016	PASS
75	95	30	80	49.5	8529	PASS
95	95	100	100	100.0	17242	PASS
96	95	5	9	6.6	1138	PASS
173	174	0.00	2	0.4	46	PASS
174	95	50	120	62.0	10690	PASS
175	174	5	9	6.8	728	PASS
176	174	95	101	97.6	10432	PASS
177	176	5	9	6.6	684	PASS

m/z	Abundance
35.90	130.0
36.90	810.0
38.00	649.0
39.00	296.0
43.00	103.0
43.90	347.0
45.00	156.0
47.00	202.0
47.80	122.0
48.90	687.0
50.00	3018.0
51.00	1042.0
55.10	128.0
55.90	281.0
56.90	457.0
59.90	160.0
61.00	725.0
62.00	761.0
62.90	507.0
68.00	1764.0
69.00	1825.0
70.00	130.0
73.00	758.0
74.00	2730.0
75.00	8411.0
76.00	741.0
78.80	461.0
79.90	140.0
80.90	408.0
81.90	145.0
86.90	600.0
87.90	613.0
91.80	470.0
93.00	667.0
94.00	1767.0
95.00	16584.0
96.00	1022.0
116.90	108.0
140.80	183.0
142.90	145.0
174.00	10089.0
174.90	697.0
175.90	9837.0
176.90	660.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
35.90	130.0
37.00	821.0
37.90	725.0
39.00	311.0
43.00	100.0
43.90	346.0
45.00	163.0
47.00	210.0
47.90	146.0
48.90	713.0
50.00	3104.0
51.00	1063.0
55.00	142.0
55.90	272.0
56.90	530.0
60.00	161.0
61.00	812.0
62.00	804.0
63.00	536.0
68.00	1833.0
69.00	1916.0
70.00	147.0
73.00	757.0
74.00	2907.0
75.00	8960.0
76.00	768.0
76.90	105.0
77.90	105.0
78.80	495.0
79.90	143.0
80.90	412.0
81.80	134.0
86.90	607.0
87.90	599.0
91.80	442.0
93.00	738.0
94.00	1977.0
95.00	17920.0
96.00	1193.0
116.90	121.0
140.80	193.0
142.90	179.0
174.00	11080.0
174.90	723.0
175.90	10835.0
176.90	714.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
36.00	135.0
37.00	740.0
37.90	749.0
38.90	305.0
39.80	112.0
40.90	104.0
43.90	374.0
45.00	170.0
47.00	192.0
47.90	142.0
48.90	646.0
50.00	2927.0
51.00	964.0
55.10	137.0
55.90	254.0
56.90	543.0
60.00	152.0
61.00	763.0
62.00	771.0
63.00	510.0
68.00	1702.0
69.00	1804.0
69.90	164.0
73.00	650.0
74.00	2740.0
75.00	8216.0
76.00	741.0
76.90	129.0
78.80	474.0
79.90	130.0
80.90	410.0
81.80	121.0
86.90	604.0
87.90	540.0
91.80	387.0
93.00	729.0
94.00	2039.0
95.00	17224.0
96.00	1201.0
116.90	106.0
140.80	178.0
142.90	188.0
173.00	140.0
173.90	10902.0
174.90	765.0
175.90	10624.0
176.90	679.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
39.90	110.0
43.90	370.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49