

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102419\
 Data File : VV013316.D
 Acq On : 24 Oct 2019 14:11
 Operator : SY/MD
 Sample : VV1024WBL01
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	87	rVB	546852	572903	11.48%	1.571%
2	1.579	145	152	164	rBV	474724	528706	10.59%	1.450%
3	2.123	313	321	332	rVB	895964	1235423	24.75%	3.389%
4	3.142	636	638	641	rBV2	1515	713	0.01%	0.002%
5	3.196	650	655	656	rBV3	2136	1324	0.03%	0.004%
6	3.335	696	698	701	rBV3	1720	1153	0.02%	0.003%
7	3.373	705	710	713	rBV4	2291	1852	0.04%	0.005%
8	3.441	725	731	733	rBV5	1329	1394	0.03%	0.004%
9	3.499	747	749	750	rBV2	1274	554	0.01%	0.002%
10	3.528	756	758	760	rVB2	1057	405	0.01%	0.001%
11	3.544	760	763	764	rBV2	1064	521	0.01%	0.001%
12	3.582	773	775	778	rBV3	648	439	0.01%	0.001%
13	3.631	787	790	792	rVB3	1744	771	0.02%	0.002%
14	3.643	792	794	796	rBV2	805	454	0.01%	0.001%
15	3.663	798	800	801	rBV2	343	103	0.00%	0.000%
16	3.682	805	806	808	rBV2	837	422	0.01%	0.001%
17	3.743	821	825	829	rBV7	1285	834	0.02%	0.002%
18	3.769	829	833	835	rVB5	1193	869	0.02%	0.002%
19	3.785	835	838	839	rBV2	753	392	0.01%	0.001%
20	3.811	844	846	848	rBV3	669	437	0.01%	0.001%
21	3.827	850	851	853	rBV2	476	184	0.00%	0.001%
22	3.846	853	857	858	rBV3	814	515	0.01%	0.001%
23	3.865	861	863	865	rVB3	922	374	0.01%	0.001%
24	3.888	867	870	871	rBV3	1211	709	0.01%	0.002%
25	3.962	879	893	948	rBV	179906	1040315	20.84%	2.854%
26	4.393	1013	1027	1059	rVB	801025	1945606	38.98%	5.337%
27	4.817	1156	1159	1160	rBV3	791	464	0.01%	0.001%
28	4.991	1210	1213	1216	rBV3	1565	1211	0.02%	0.003%
29	5.087	1224	1243	1282	rBV2	2017216	4990828	100.00%	13.689%
30	5.511	1372	1375	1376	rBV3	1776	1144	0.02%	0.003%
31	5.656	1406	1420	1453	rBV	1525481	3026985	60.65%	8.303%
32	5.946	1499	1510	1530	rVB3	54775	111470	2.23%	0.306%
33	6.113	1547	1562	1589	rBV	1087252	2237408	44.83%	6.137%
34	6.360	1637	1639	1643	rVB5	1525	957	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102419\
 Data File : VV013316.D
 Acq On : 24 Oct 2019 14:11
 Operator : SY/MD
 Sample : VV1024WBL01
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
 Title : VOC Analysis

35	6.473	1671	1674	1680	rBV6	1772	1556	0.03%	0.004%
36	6.521	1687	1689	1690	rBV2	1402	628	0.01%	0.002%
37	6.540	1693	1695	1701	rVV6	1612	1838	0.04%	0.005%
38	6.618	1716	1719	1723	rBV6	1160	1012	0.02%	0.003%
39	6.765	1763	1765	1768	rBV3	1487	1025	0.02%	0.003%
40	6.791	1771	1773	1776	rVB3	1081	689	0.01%	0.002%
41	6.820	1780	1782	1783	rBV2	1148	468	0.01%	0.001%
42	6.855	1790	1793	1794	rBV2	634	331	0.01%	0.001%
43	6.865	1794	1796	1797	rBV2	796	390	0.01%	0.001%
44	6.891	1803	1804	1805	rBV	764	238	0.00%	0.001%
45	6.904	1805	1808	1810	rVB3	769	432	0.01%	0.001%
46	6.939	1817	1819	1821	rBV4	923	433	0.01%	0.001%
47	6.971	1827	1829	1831	rBV3	621	243	0.00%	0.001%
48	7.023	1831	1845	1868	rBV	595463	1088586	21.81%	2.986%
49	7.354	1935	1948	1969	rBV	2379531	4050205	81.15%	11.109%
50	7.659	2029	2043	2066	rBV	413319	730037	14.63%	2.002%
51	7.958	2134	2136	2138	rBV3	1788	1148	0.02%	0.003%
52	8.135	2179	2191	2226	rBV2	1014022	2324607	46.58%	6.376%
53	8.740	2376	2379	2380	rBV2	778	455	0.01%	0.001%
54	8.814	2400	2402	2403	rBV2	1424	767	0.02%	0.002%
55	8.891	2414	2426	2446	rBV	2256675	3596148	72.06%	9.864%
56	9.254	2537	2539	2541	rBV2	1039	495	0.01%	0.001%
57	9.412	2586	2588	2590	rBV3	1151	611	0.01%	0.002%
58	9.466	2598	2605	2606	rBV8	1148	1319	0.03%	0.004%
59	9.608	2637	2649	2659	rVB9	6322	15251	0.31%	0.042%
60	9.695	2670	2676	2679	rBV6	1461	1675	0.03%	0.005%
61	9.743	2687	2691	2692	rBV3	1106	848	0.02%	0.002%
62	9.765	2695	2698	2702	rBV4	1681	1654	0.03%	0.005%
63	9.804	2708	2710	2711	rBV	1141	419	0.01%	0.001%
64	9.852	2722	2725	2728	rBV5	1363	1201	0.02%	0.003%
65	9.875	2730	2732	2734	rBV2	621	313	0.01%	0.001%
66	9.936	2749	2751	2753	rBV2	1233	709	0.01%	0.002%
67	10.039	2781	2783	2784	rBV2	473	163	0.00%	0.000%
68	10.048	2784	2786	2789	rVV3	941	398	0.01%	0.001%
69	10.119	2804	2808	2810	rBV5	2393	2054	0.04%	0.006%
70	10.187	2826	2829	2830	rBV3	1002	431	0.01%	0.001%
71	10.257	2838	2851	2874	rBV	1485432	2343854	46.96%	6.429%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102419\
 Data File : VV013316.D
 Acq On : 24 Oct 2019 14:11
 Operator : SY/MD
 Sample : VV1024WBL01
 Misc : 5.00ML/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
 Title : VOC Analysis

72	10.482	2917	2921	2923	rBV3	1353	1011	0.02%	0.003%
73	10.543	2934	2940	2941	rBV6	1800	1713	0.03%	0.005%
74	10.553	2941	2943	2945	rVV3	1534	984	0.02%	0.003%
75	10.585	2945	2953	2963	rVB10	4472	9419	0.19%	0.026%
76	10.643	2968	2971	2974	rBV5	1268	813	0.02%	0.002%
77	10.662	2976	2977	2980	rBV2	1194	746	0.01%	0.002%
78	10.701	2986	2989	2993	rBV5	1770	1206	0.02%	0.003%
79	10.762	3006	3008	3009	rBV2	1120	463	0.01%	0.001%
80	10.801	3016	3020	3023	rBV5	877	871	0.02%	0.002%
81	10.955	3061	3068	3074	rBV4	6188	8659	0.17%	0.024%
82	11.016	3085	3087	3090	rBV3	1060	663	0.01%	0.002%
83	11.035	3090	3093	3095	rBV4	1074	644	0.01%	0.002%
84	11.129	3117	3122	3123	rBV3	1653	1636	0.03%	0.004%
85	11.225	3141	3152	3159	rBV3	12158	22011	0.44%	0.060%
86	11.289	3160	3172	3193	rVV	2003319	3053944	61.19%	8.377%
87	11.666	3276	3289	3316	rBV	2215895	3467393	69.48%	9.511%
88	12.042	3404	3406	3408	rBV3	1778	860	0.02%	0.002%
89	12.132	3432	3434	3436	rBV3	919	417	0.01%	0.001%
90	12.421	3520	3524	3526	rBV4	1701	1503	0.03%	0.004%
91	12.563	3565	3568	3572	rBV6	2596	2023	0.04%	0.006%


Sum of corrected areas: 36457449

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102419\
Data File : VV013316.D
Acq On : 24 Oct 2019 14:11
Operator : SY/MD
Sample : VV1024WBL01
Misc : 5.00ML/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

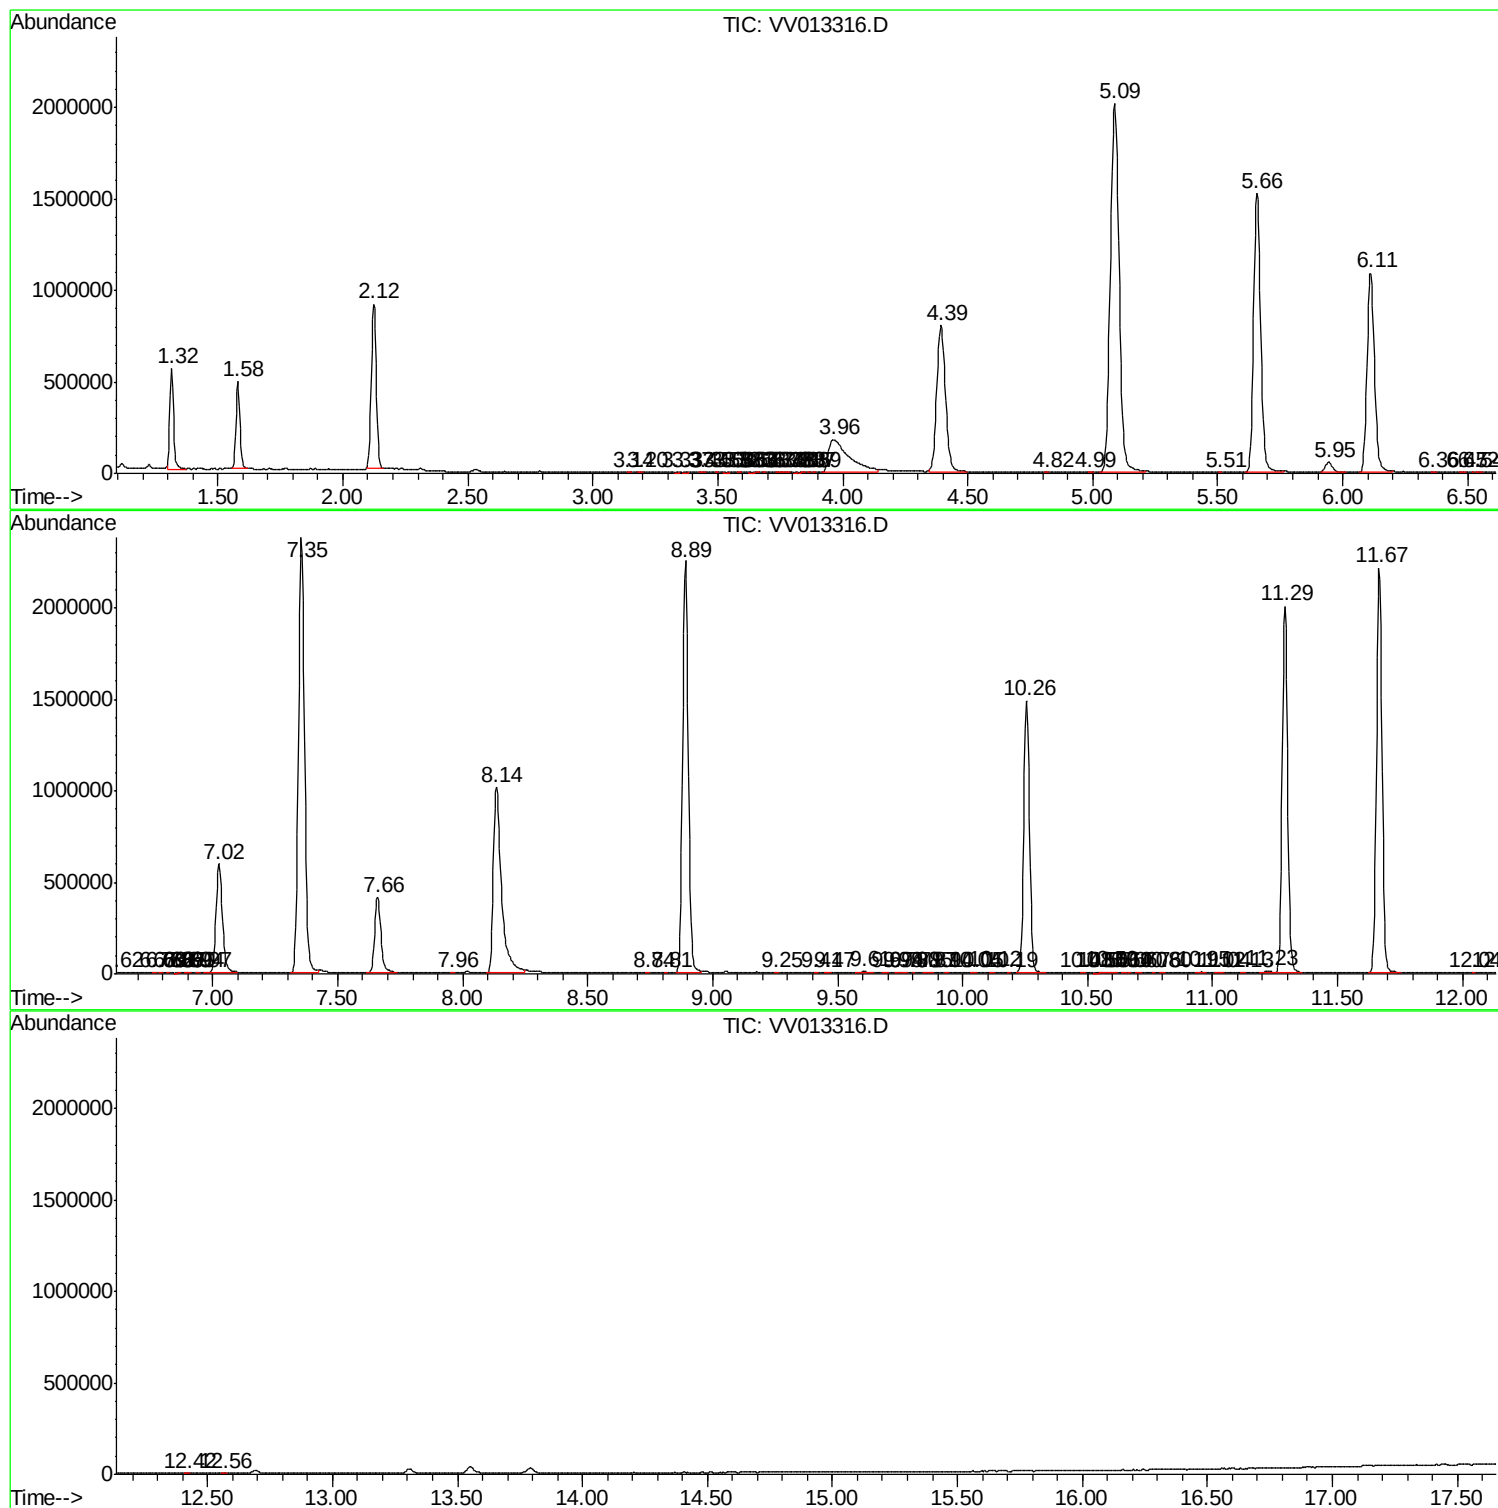

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102419\
Data File : VV013316.D
Acq On : 24 Oct 2019 14:11
Operator : SY/MD
Sample : VV1024WBL01
Misc : 5.00ML/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV102419\
Data File : VV013316.D
Acq On : 24 Oct 2019 14:11
Operator : SY/MD
Sample : VV1024WBL01
Misc : 5.00ML/MSV0A_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc