


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV102419\
Data File : VV013314.D
Acq On : 24 Oct 2019 13:04
Operator : SY/MD
Sample : BFB75
Misc : 5.00ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB75

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102319WMA.M
Title : VOC Analysis
Last Update : Fri Oct 25 13:28:06 2019

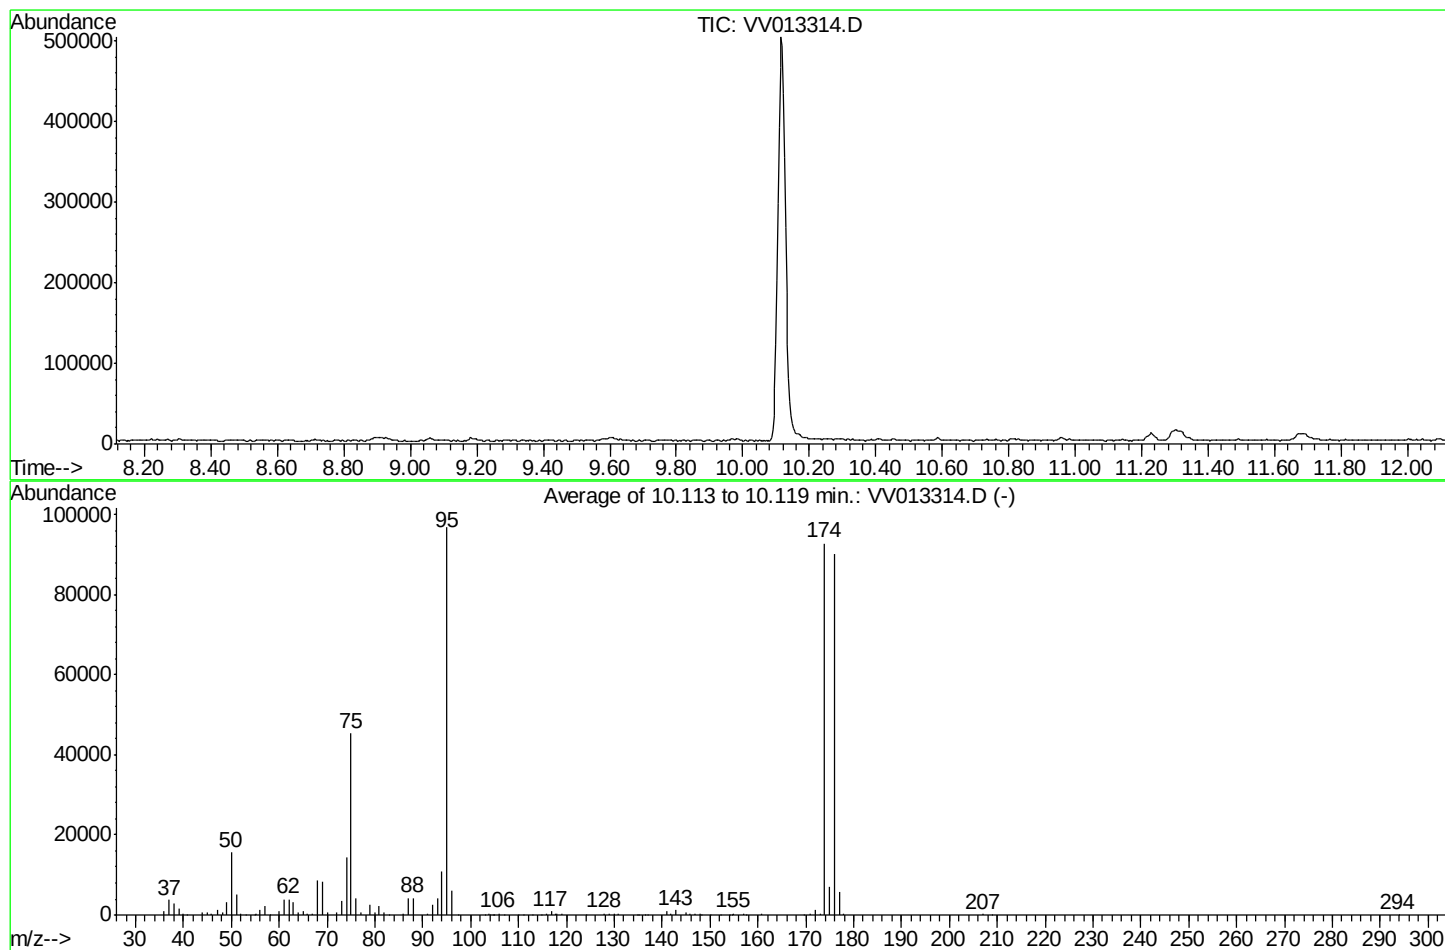

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	15527	PASS
75	95	30	80	46.8	45320	PASS
95	95	100	100	100.0	96768	PASS
96	95	5	9	6.3	6132	PASS
173	174	0.00	2	0.4	413	PASS
174	95	50	120	95.9	92792	PASS
175	174	5	9	7.4	6890	PASS
176	174	95	101	97.2	90194	PASS
177	176	5	9	6.4	5763	PASS

m/z	Abundance
36.00	846.0
37.00	3459.0
38.00	3235.0
39.00	1608.0
40.00	1694.0
40.80	194.0
42.10	119.0
43.00	137.0
44.00	1715.0
45.00	762.0
45.90	130.0
47.10	1083.0
48.10	553.0
49.00	3095.0
50.10	15330.0
51.00	5163.0
52.10	321.0
55.10	389.0
56.00	1350.0
57.00	2234.0
58.00	133.0
59.90	1032.0
61.00	3855.0
62.00	4047.0
63.00	3267.0
64.00	593.0
65.00	930.0
65.90	219.0
67.00	218.0
68.00	8299.0
69.00	8199.0
70.00	755.0
71.90	512.0
73.00	3556.0
74.00	13284.0
75.00	44264.0
76.00	3785.0
77.10	653.0
78.90	2381.0
79.90	695.0
80.90	2369.0
82.00	623.0
85.80	171.0
86.90	3724.0
88.00	4206.0
90.90	400.0
92.10	2283.0
93.00	3639.0
94.00	10501.0
95.00	92248.0
96.00	6468.0
97.20	174.0
102.90	108.0
103.70	243.0
104.10	222.0
104.70	238.0
105.90	355.0
106.90	151.0
109.90	127.0
111.00	126.0
114.80	118.0
115.80	340.0
116.90	832.0
118.00	337.0
119.00	430.0
127.90	443.0
128.90	302.0
129.90	272.0
130.80	178.0
134.80	147.0
136.80	148.0
140.90	870.0
141.80	202.0
142.90	1233.0
145.00	560.0
145.90	263.0
146.90	169.0
147.90	322.0
150.10	166.0
152.10	110.0
154.20	194.0
154.70	248.0
155.00	276.0
157.00	175.0
160.90	204.0
170.80	211.0
171.90	1338.0
173.90	87640.0
175.00	6411.0
176.00	84856.0
177.00	5573.0
178.00	259.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

207.00
293.80

159.0
141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	915.0
37.00	3920.0
38.00	3314.0
39.00	1647.0
39.90	1609.0
40.70	139.0
42.10	114.0
43.00	149.0
44.00	1692.0
45.00	841.0
45.90	224.0
47.00	1235.0
48.00	656.0
49.00	3374.0
50.10	16094.0
51.00	5442.0
52.00	325.0
53.10	142.0
55.10	324.0
55.90	1229.0
57.10	2151.0
58.10	169.0
59.90	1084.0
61.00	4043.0
62.00	3987.0
63.00	3338.0
64.00	689.0
64.90	810.0
65.90	228.0
67.00	237.0
68.00	8999.0
69.10	8609.0
70.00	755.0
71.90	526.0
73.00	3521.0
74.10	14924.0
75.00	47056.0
76.00	4187.0
77.10	693.0
78.90	2833.0
79.90	735.0
80.90	2443.0
82.00	580.0
85.80	215.0
87.00	4140.0
88.00	4521.0
90.90	397.0
92.10	2585.0
93.00	4286.0
94.00	11065.0
95.00	99928.0
96.00	6335.0
97.30	174.0
102.90	126.0
103.70	310.0
104.70	212.0
105.90	426.0
106.90	163.0
110.00	109.0
111.00	115.0
115.90	412.0
116.90	919.0
117.70	302.0
118.10	396.0
119.00	483.0
124.00	116.0
127.90	475.0
128.80	297.0
129.90	305.0
130.90	218.0
134.80	162.0
136.30	110.0
136.80	182.0
140.90	952.0
141.90	194.0
142.90	1242.0
145.00	627.0
145.90	226.0
146.80	194.0
147.90	235.0
150.10	153.0
152.10	129.0
154.10	155.0
154.90	437.0
156.90	245.0
157.50	110.0
160.80	253.0
170.80	257.0
171.80	1441.0
173.90	95968.0
175.00	7164.0
176.00	93088.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

177.00	5910.0
177.90	311.0
207.00	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

m/z	Abundance
36.00	1010.0
37.00	3986.0
38.00	3019.0
39.00	1480.0
39.90	1473.0
43.00	113.0
44.00	1780.0
44.90	818.0
45.90	277.0
47.00	1270.0
48.00	613.0
49.00	3276.0
50.00	15158.0
51.00	5161.0
52.00	261.0
53.10	203.0
54.80	170.0
55.20	206.0
55.90	1071.0
57.10	1897.0
58.10	143.0
59.90	953.0
61.00	3690.0
62.10	3868.0
63.00	3230.0
64.00	670.0
64.90	759.0
65.90	181.0
67.00	215.0
68.00	8634.0
69.00	8044.0
70.00	675.0
72.00	598.0
73.00	3288.0
74.00	14894.0
75.00	44640.0
76.00	4106.0
77.10	650.0
78.90	2961.0
79.90	777.0
80.90	2390.0
81.90	507.0
83.00	136.0
85.90	190.0
87.00	4396.0
88.00	3942.0
90.90	306.0
92.00	2474.0
93.00	4356.0
94.00	10670.0
95.00	98128.0
96.00	5595.0
97.30	105.0
102.90	126.0
103.70	306.0
104.90	214.0
105.90	382.0
106.90	134.0
113.00	122.0
115.90	410.0
116.90	873.0
117.70	307.0
118.10	370.0
119.00	526.0
124.00	105.0
127.90	484.0
128.80	211.0
129.90	288.0
131.00	201.0
135.00	149.0
136.90	183.0
140.90	962.0
141.90	137.0
142.90	1099.0
145.00	639.0
145.90	175.0
146.80	191.0
147.80	157.0
148.10	152.0
150.10	111.0
154.00	123.0
154.90	489.0
156.90	291.0
157.50	108.0
160.80	231.0
169.60	130.0
170.80	272.0
171.80	1459.0
173.10	1240.0
173.90	94768.0
174.90	7096.0
176.00	92640.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

177.00	5808.0
177.90	310.0
207.10	197.0
209.00	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75

Scan 2794 (10.074 min): VV013314.D
BFB75

m/z	Abundance
35.40	112.0
37.90	205.0
39.90	1329.0
42.30	219.0
42.90	143.0
43.30	154.0
44.00	1060.0
64.20	154.0
78.10	123.0
107.00	113.0
216.10	132.0
269.00	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB75