




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032610.D
Acq On : 24 Oct 2023 23:46
Operator : SY/MD
Sample : 04995-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4941

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/25/2023
Supervised By :Mahesh Dadoda 10/26/2023

Quant Time: Oct 25 08:35:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 25 08:15:09 2023
Response via : Initial Calibration

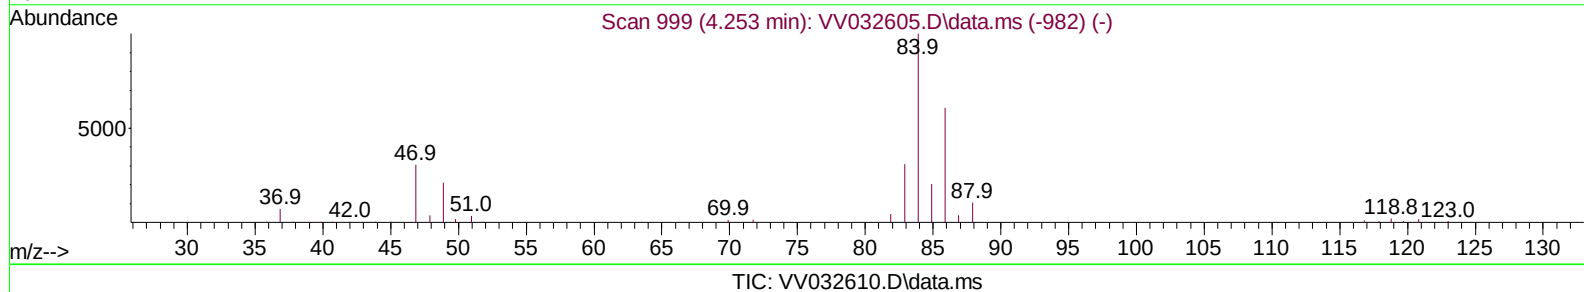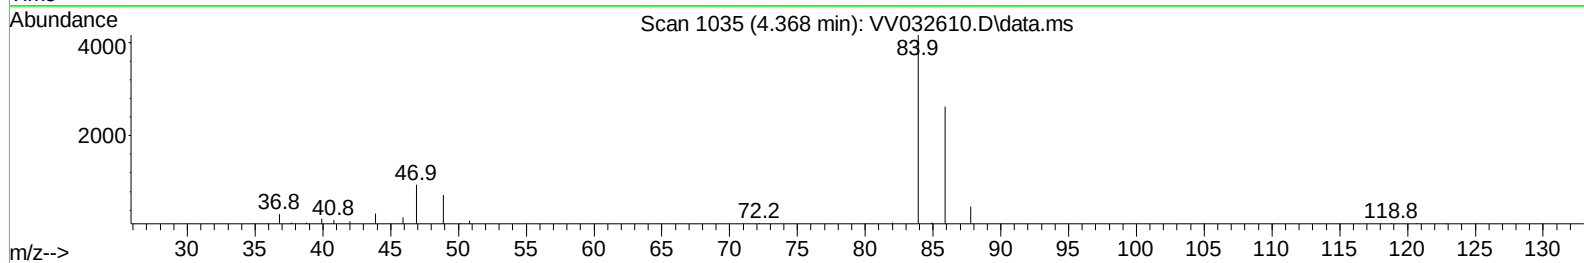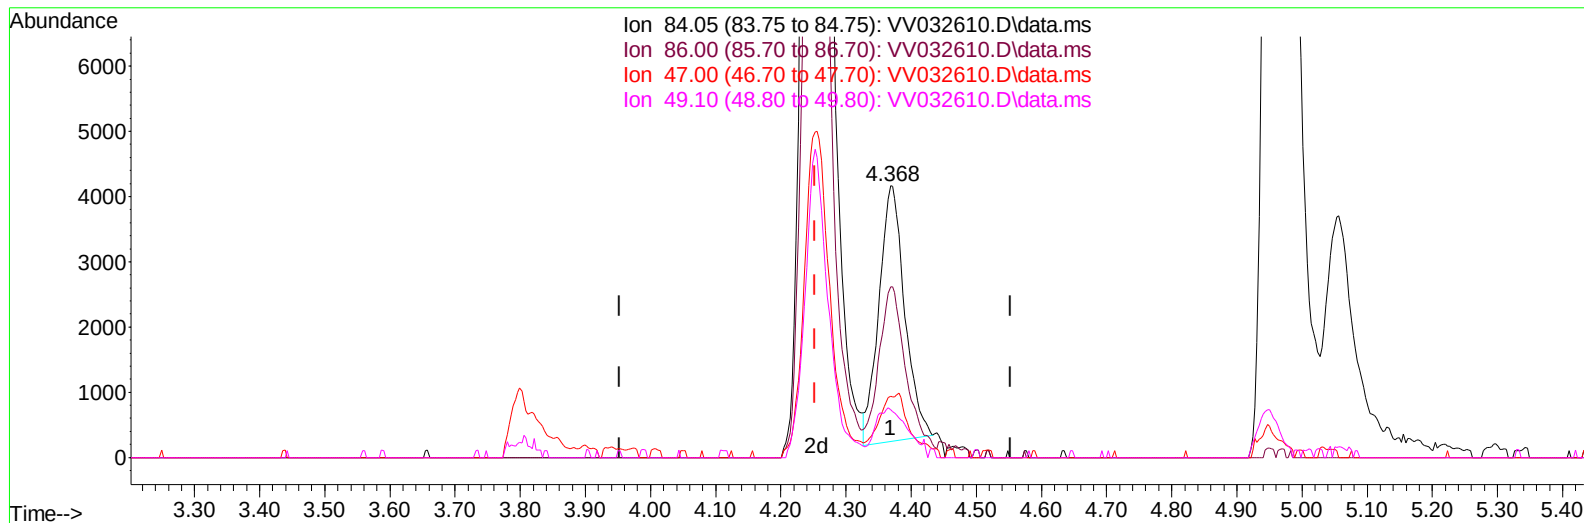

(24) Chloroform-d (S)

4.368min (+ 0.116) 0.81 ug/L

response 10746

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	61.90	67.76
47.00	43.10	31.12
49.10	25.00	24.56




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032610.D
Acq On : 24 Oct 2023 23:46
Operator : SY/MD
Sample : 04995-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4941

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/25/2023
Supervised By :Mahesh Dadoda 10/26/2023

Quant Time: Oct 25 08:35:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 25 08:15:09 2023
Response via : Initial Calibration

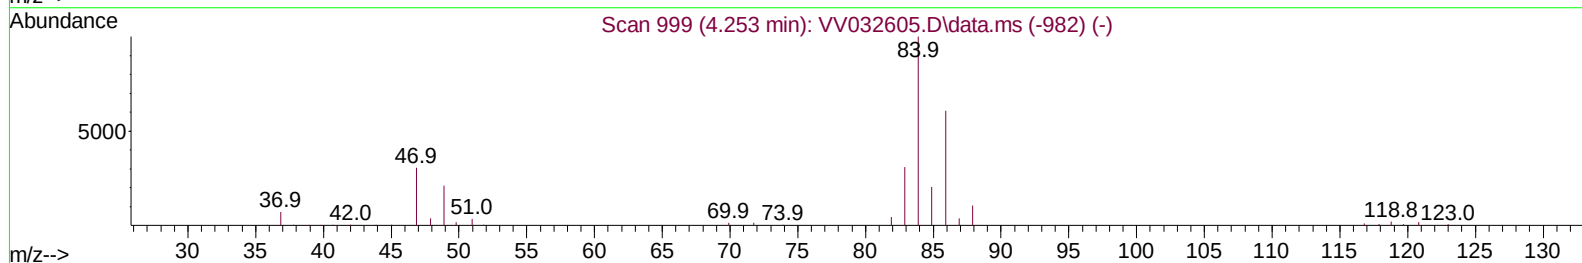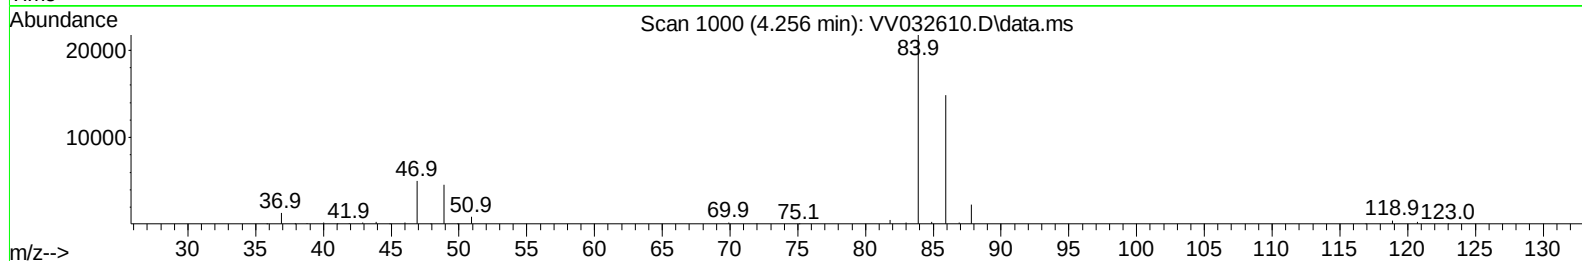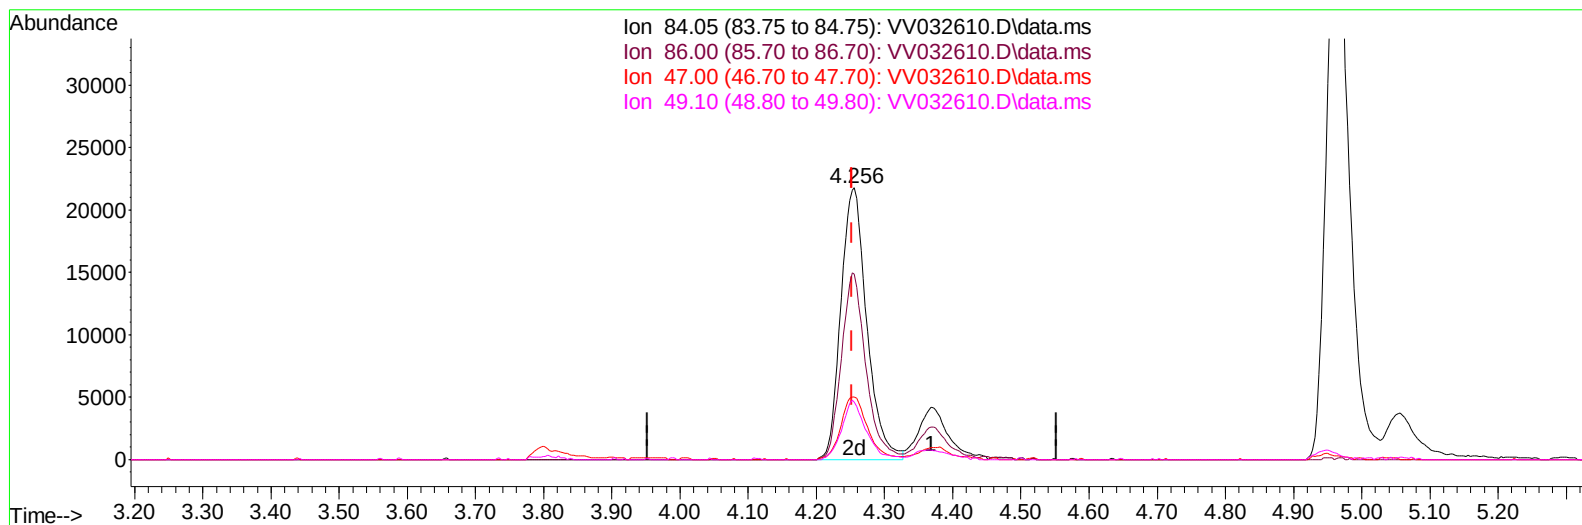

TIC: VV032610.D\data.ms

(24) Chloroform-d (S)

4.256min (+ 0.003) 4.29 ug/L m

response 57196

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	61.90	12.73#
47.00	43.10	5.85#
49.10	25.00	4.61#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032610.D
Acq On : 24 Oct 2023 23:46
Operator : SY/MD
Sample : 04995-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4941

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/25/2023
Supervised By :Mahesh Dadoda 10/26/2023

Quant Time: Oct 25 08:35:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 25 08:15:09 2023
Response via : Initial Calibration

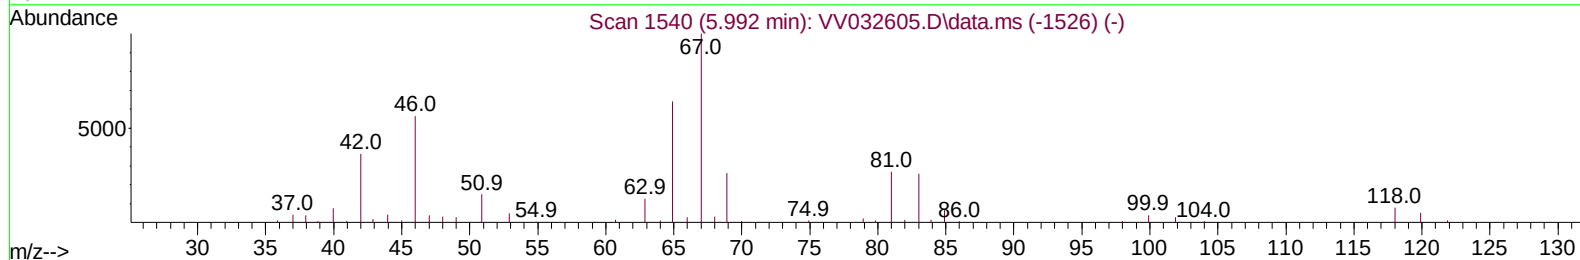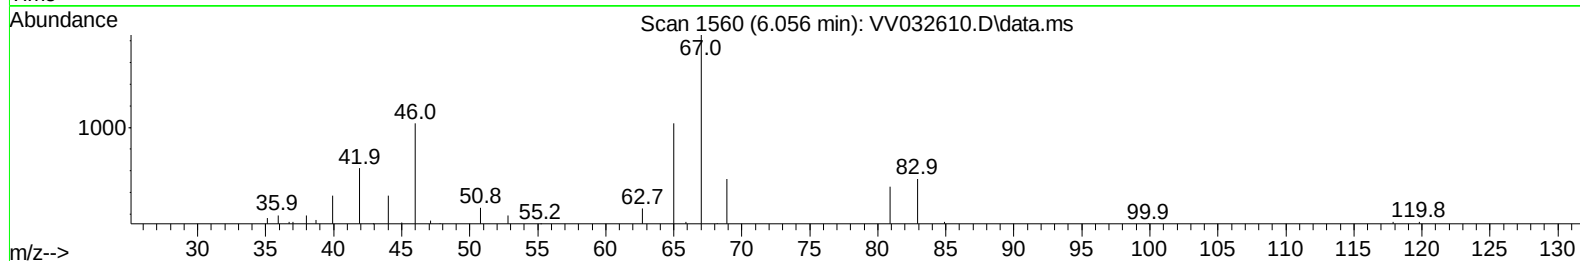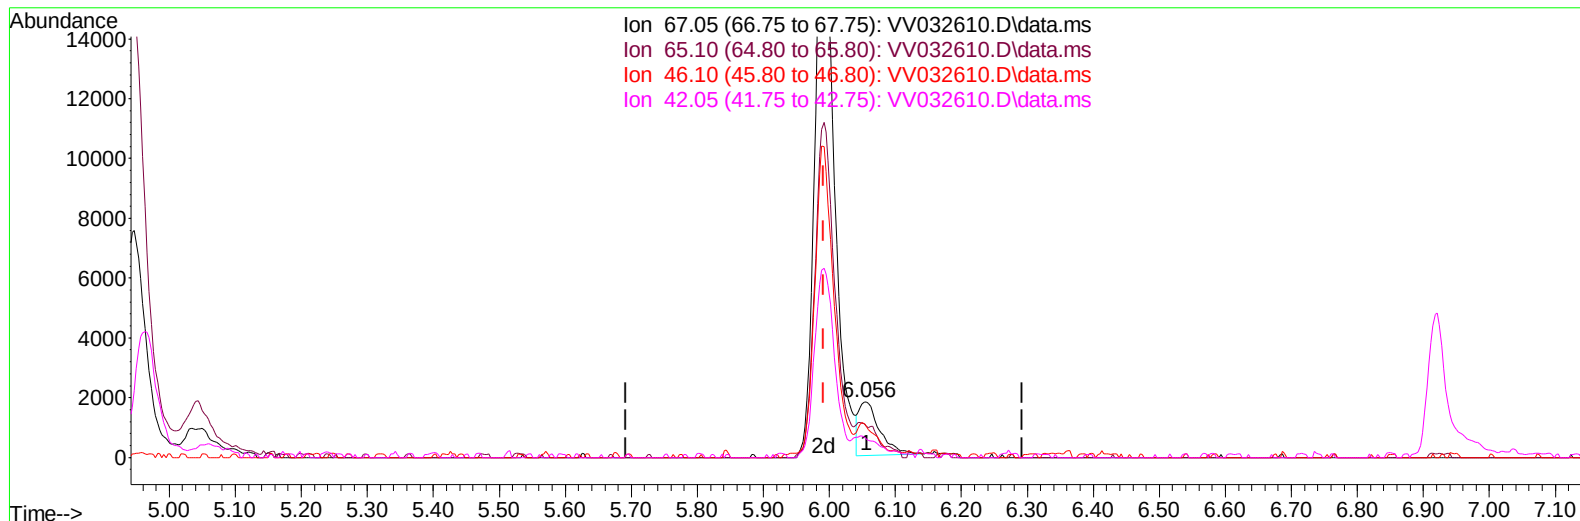

TIC: VV032610.D\data.ms

(36) 1,2-Dichloropropane-d6 (S)

6.056min (+ 0.064) 0.39 ug/L

response 3975

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	67.60	73.01
46.10	49.60	52.68
42.05	26.30	32.88




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
 Data File : VV032610.D
 Acq On : 24 Oct 2023 23:46
 Operator : SY/MD
 Sample : 04995-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4941

Manual IntegrationsAPPROVED

Quant Time: Oct 25 08:35:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 25 08:15:09 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/25/2023
 Supervised By :Mahesh Dadoda 10/26/2023

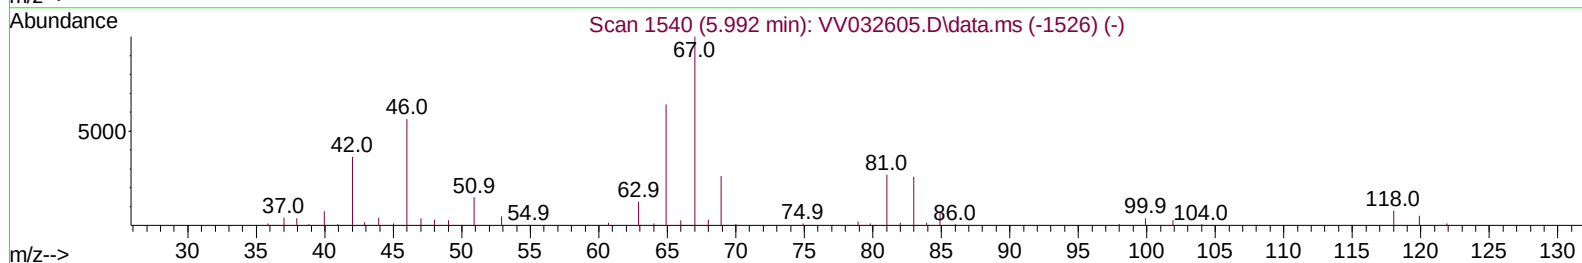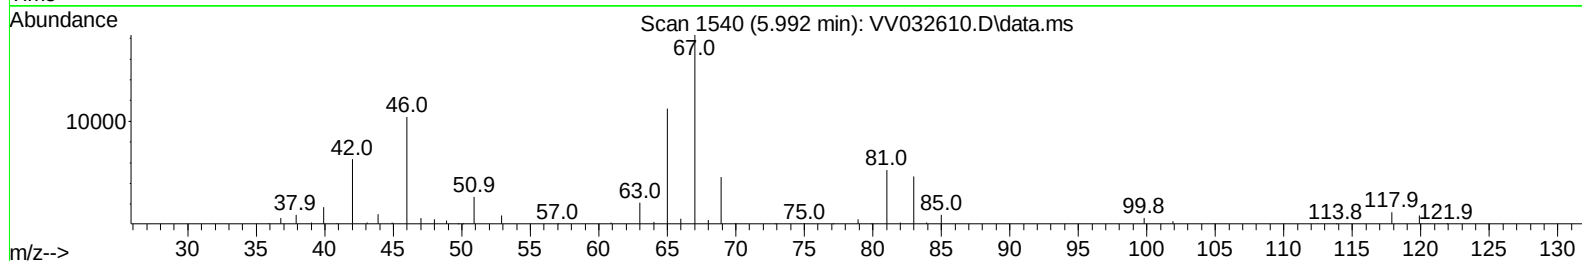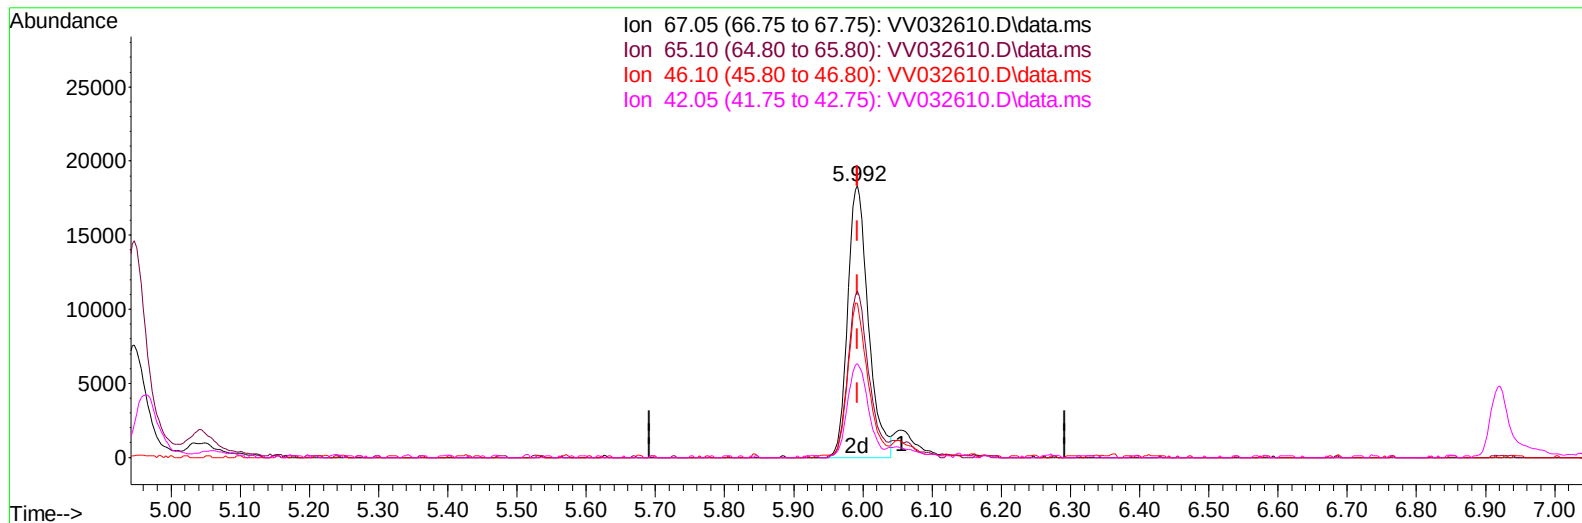

TIC: VV032610.D\data.ms

(36) 1,2-Dichloropropane-d6 (S)

5.992min (-0.000) 3.73 ug/L m

response 38286

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	67.60	7.58#
46.10	49.60	5.47#
42.05	26.30	3.41#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
 Data File : VV032610.D
 Acq On : 24 Oct 2023 23:46
 Operator : SY/MD
 Sample : 04995-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4941

Manual IntegrationsAPPROVED

Quant Time: Oct 25 08:35:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 25 08:15:09 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/25/2023
 Supervised By :Mahesh Dadoda 10/26/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		92831	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117		105251	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		46487	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		24014	3.181	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	63.600%	
7) Chloroethane-d5	1.532	69		27749	4.528	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.600%	
11) 1,1-Dichloroethene-d2	2.060	65		9113	2.862	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.200%#	
20) 2-Butanone-d5	3.796	46		103147	54.008	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.020%	
24) Chloroform-d	4.256	84		57196m	4.294	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.800%	
26) 1,2-Dichloroethane-d4	4.947	65		33059	5.240	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.800%	
32) Benzene-d6	4.963	84		104036	3.359	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	67.200%#	
36) 1,2-Dichloropropane-d6	5.992	67		38286m	3.731	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	74.600%	
41) Toluene-d8	7.246	98		86718	3.062	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	61.200%#	
43) trans-1,3-Dichloroprop...	7.561	79		13877	3.816	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.400%	
46) 2-Hexanone-d5	8.027	63		85066	49.723	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.440%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84		36321	5.061	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.200%	
66) 1,2-Dichlorobenzene-d4	11.564	152		38234	4.432	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.600%	
Target Compounds							
3) Chloromethane	1.217	50		3045	0.292	ug/L	98
13) Acetone	2.130	43		2284	1.552	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032610.D
Acq On : 24 Oct 2023 23:46
Operator : SY/MD
Sample : 04995-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4941

Manual IntegrationsAPPROVED

Quant Time: Oct 25 08:35:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 25 08:15:09 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/25/2023
Supervised By :Mahesh Dadoda 10/26/2023

