

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
 Data File : VV032615.D
 Acq On : 25 Oct 2023 01:47
 Operator : SY/MD
 Sample : 04995-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49C3

Quant Time: Oct 25 08:36:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 25 08:15:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	85379	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	97411	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	42284	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	21164	3.048	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	61.000%	
7) Chloroethane-d5	1.532	69	25069	4.448	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	89.000%	
11) 1,1-Dichloroethene-d2	2.060	65	8174	2.791	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	55.800%#	
20) 2-Butanone-d5	3.799	46	90083	51.284	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	102.560%	
24) Chloroform-d	4.253	84	49663	4.054	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	81.000%	
26) 1,2-Dichloroethane-d4	4.947	65	28577	4.925	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.600%	
32) Benzene-d6	4.963	84	91669	3.198	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	64.000%#	
36) 1,2-Dichloropropane-d6	5.989	67	32937	3.468	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	69.400%	
41) Toluene-d8	7.246	98	76458	2.917	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	58.400%#	
43) trans-1,3-Dichloroprop...	7.561	79	11701	3.477	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	69.600%	
46) 2-Hexanone-d5	8.027	63	71371	45.076	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.160%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	31691	4.771	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	95.400%	
66) 1,2-Dichlorobenzene-d4	11.564	152	33580	4.280	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	85.600%	
Target Compounds						Qvalue
13) Acetone	2.124	43	2103	1.553	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032615.D
Acq On : 25 Oct 2023 01:47
Operator : SY/MD
Sample : 04995-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49C3

Quant Time: Oct 25 08:36:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 25 08:15:09 2023
Response via : Initial Calibration

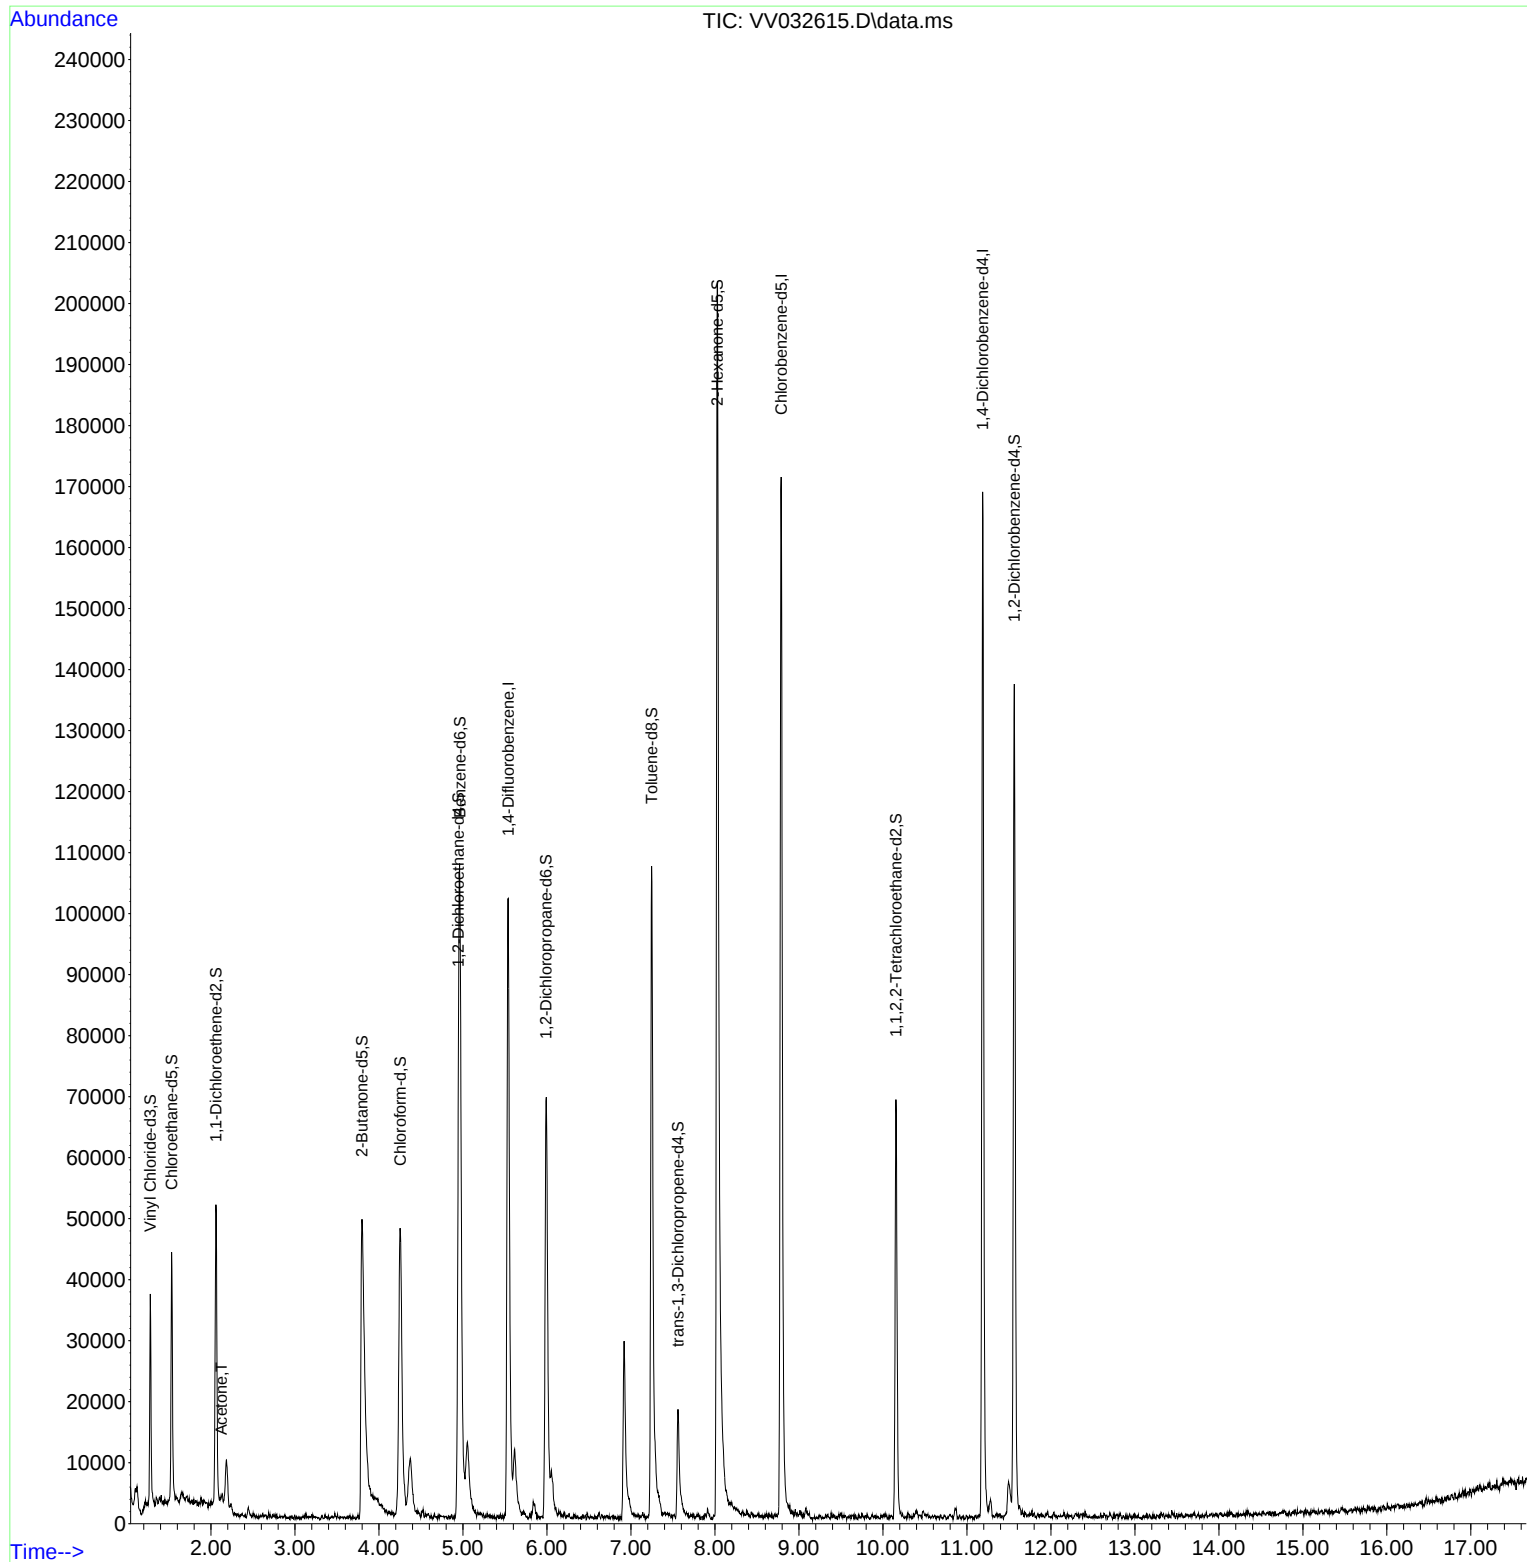

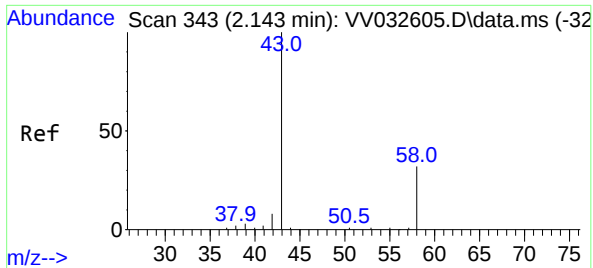

#13
 Acetone
 Concen: 1.553 ug/L
 RT: 2.124 min Scan# 31
 Delta R.T. -0.019 min
 Lab File: VV032615.D
 Acq: 25 Oct 2023 01:47

Instrument :
 MSVOA_V
 ClientSampleId :
 A49C3

Tgt Ion: 43 Resp: 2103
 Ion Ratio Lower Upper
 43 100
 58 32.2 0.0 66.0

