

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
 Data File : VV032586.D
 Acq On : 24 Oct 2023 13:35
 Operator : SY/MD
 Sample : VV1024WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK377

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	17	23	34	rVB	6003	9705	2.54%	0.315%
2	1.278	67	74	87	rVB	59236	62442	16.32%	2.029%
3	1.532	146	153	165	rBV	51398	60375	15.78%	1.962%
4	2.060	306	317	330	rBV	89115	132054	34.51%	4.292%
5	2.179	344	354	369	rVB3	13198	29872	7.81%	0.971%
6	3.825	854	866	867	rBV	23841	27990	7.32%	0.910%
7	4.253	983	999	1022	rBV2	55785	149688	39.12%	4.865%
8	4.362	1024	1033	1052	rVB4	8610	25336	6.62%	0.823%
9	4.960	1202	1219	1237	rBV3	136671	345065	90.18%	11.215%
10	5.047	1239	1246	1264	rVB4	12903	36011	9.41%	1.170%
11	5.535	1388	1398	1414	rBV	109787	231194	60.42%	7.514%
12	5.992	1527	1540	1555	rBV	80549	174232	45.53%	5.663%
13	6.918	1816	1828	1849	rBV2	34943	76228	19.92%	2.477%
14	7.246	1919	1930	1955	rBV	153272	304602	79.61%	9.900%
15	7.561	2017	2028	2043	rBV2	22628	45310	11.84%	1.473%
16	8.034	2164	2175	2212	rBV	163977	382636	100.00%	12.436%
17	8.789	2397	2410	2431	rBV	187198	334929	87.53%	10.885%
18	10.156	2825	2835	2853	rVB	64854	106175	27.75%	3.451%
19	11.188	3144	3156	3178	rBV	178389	287821	75.22%	9.354%
20	11.564	3262	3273	3296	rBV	155542	255276	66.72%	8.296%




Sum of corrected areas: 3076941

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032586.D
Acq On : 24 Oct 2023 13:35
Operator : SY/MD
Sample : VV1024WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK377

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

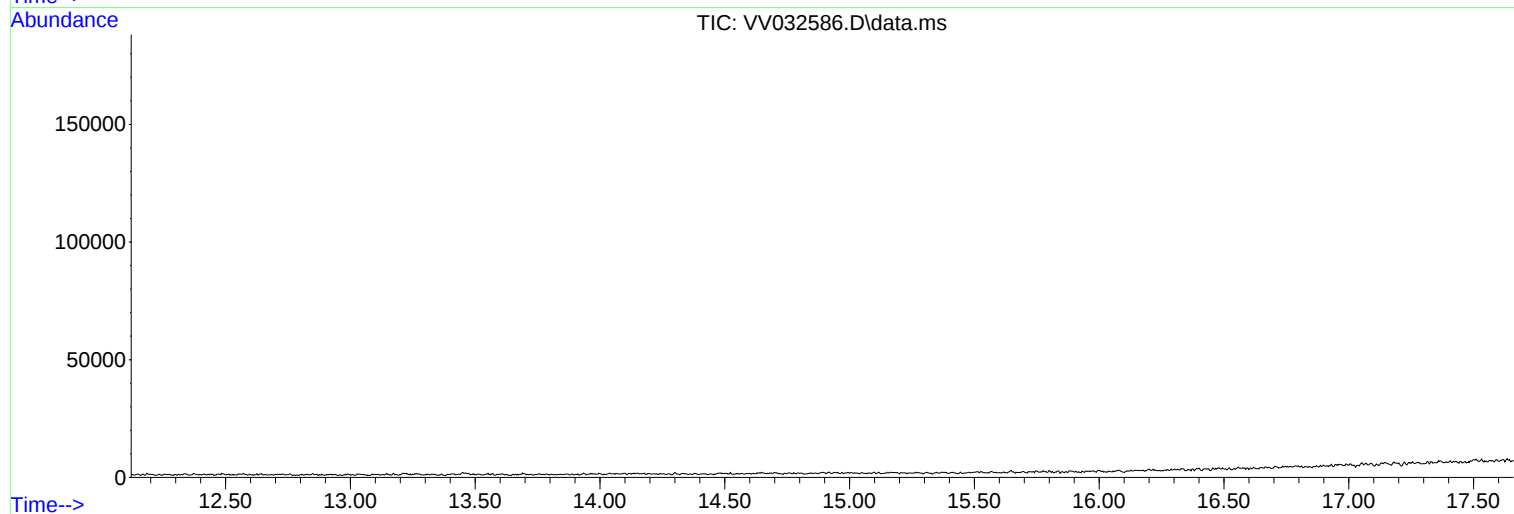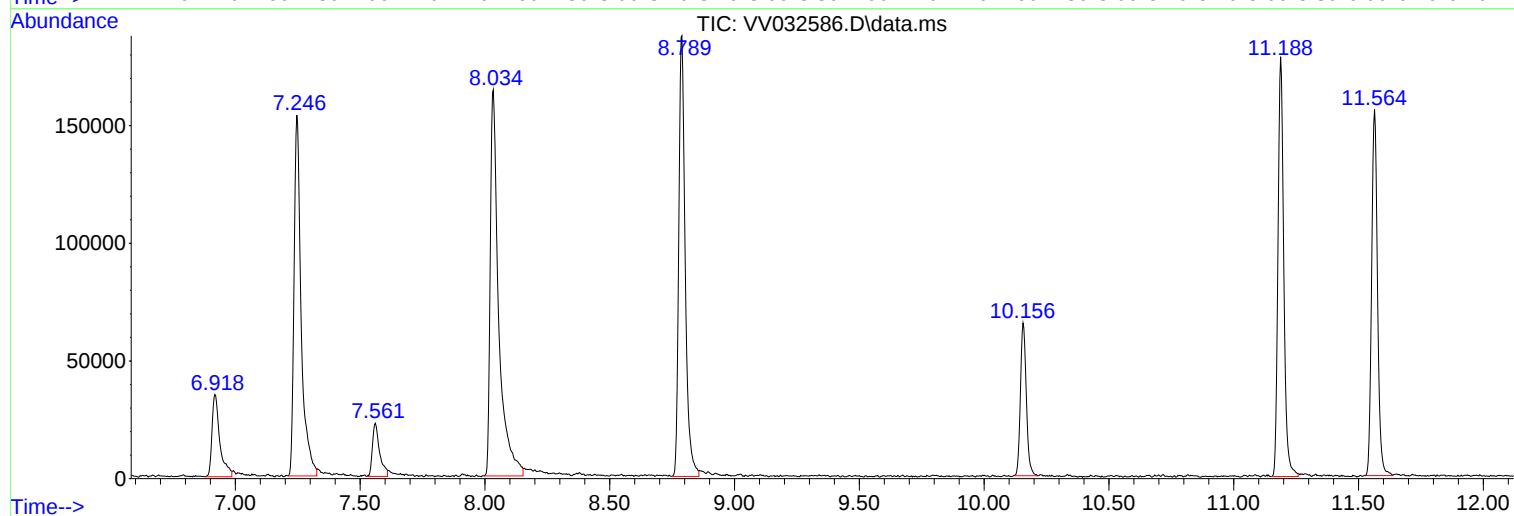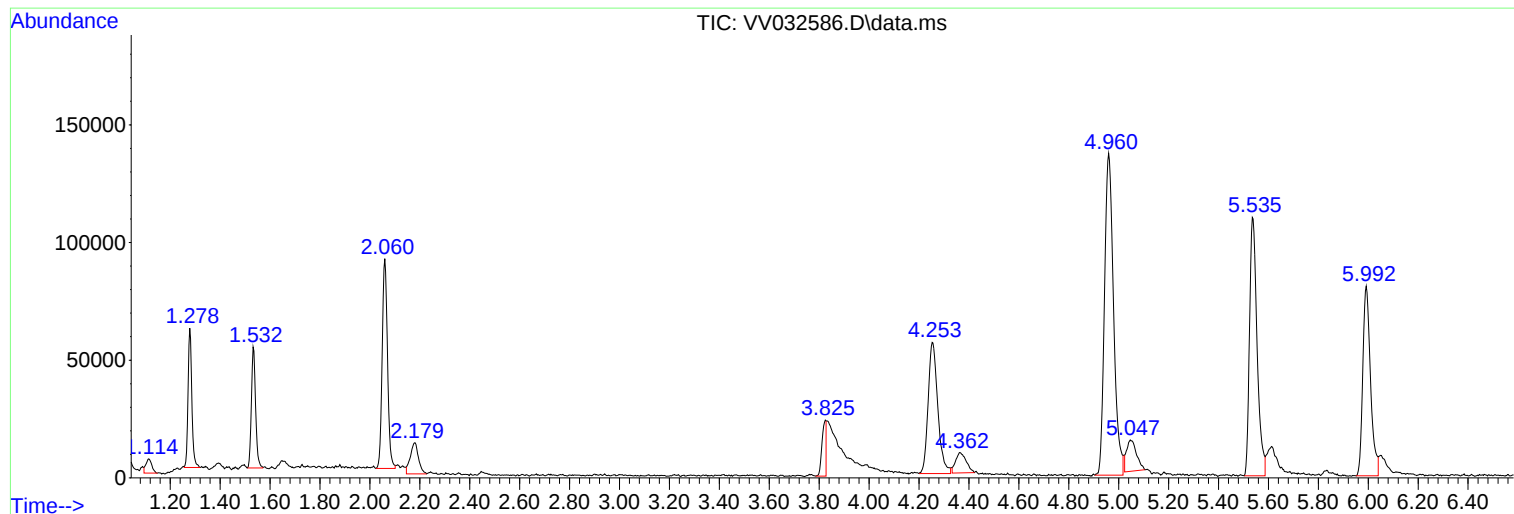

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032586.D
Acq On : 24 Oct 2023 13:35
Operator : SY/MD
Sample : VV1024WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK377

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032586.D
Acq On : 24 Oct 2023 13:35
Operator : SY/MD
Sample : VV1024WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK377

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc