

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
 Data File : VV032587.D
 Acq On : 24 Oct 2023 14:03
 Operator : SY/MD
 Sample : 04962-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COALO

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032587.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	86	rBV	37720	41539	10.26%	1.511%
2	1.532	145	153	162	rVV	40037	46529	11.49%	1.693%
3	2.059	306	317	328	rBV	56035	83449	20.60%	3.036%
4	2.178	346	354	362	rVB3	7250	13491	3.33%	0.491%
5	2.449	429	438	446	rBV7	5210	8492	2.10%	0.309%
6	3.809	852	861	891	rBV	27312	103539	25.56%	3.767%
7	3.992	909	918	937	rVB4	8229	23417	5.78%	0.852%
8	4.252	981	999	1022	rBV2	52767	156483	38.64%	5.693%
9	4.362	1025	1033	1052	rVB6	9075	27077	6.69%	0.985%
10	4.960	1200	1219	1237	rBV3	109290	286228	70.67%	10.413%
11	5.535	1386	1398	1414	rBV	98043	208206	51.41%	7.574%
12	5.992	1527	1540	1557	rBV2	70749	154384	38.12%	5.616%
13	6.918	1817	1828	1851	rBV3	27501	60425	14.92%	2.198%
14	7.246	1918	1930	1954	rBV	106687	212331	52.42%	7.725%
15	7.561	2017	2028	2052	rBV2	16572	37077	9.15%	1.349%
16	8.030	2163	2174	2206	rBV	158293	405026	100.00%	14.735%
17	8.789	2399	2410	2437	rBV	167516	299140	73.86%	10.883%
18	10.159	2825	2836	2852	rBV	65139	108470	26.78%	3.946%
19	10.332	2882	2890	2896	rBV3	3853	5438	1.34%	0.198%
20	11.188	3145	3156	3175	rBV	159859	254979	62.95%	9.276%
21	11.564	3260	3273	3293	rBV	129847	213072	52.61%	7.751%




Sum of corrected areas: 2748792

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032587.D
Acq On : 24 Oct 2023 14:03
Operator : SY/MD
Sample : 04962-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COALO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

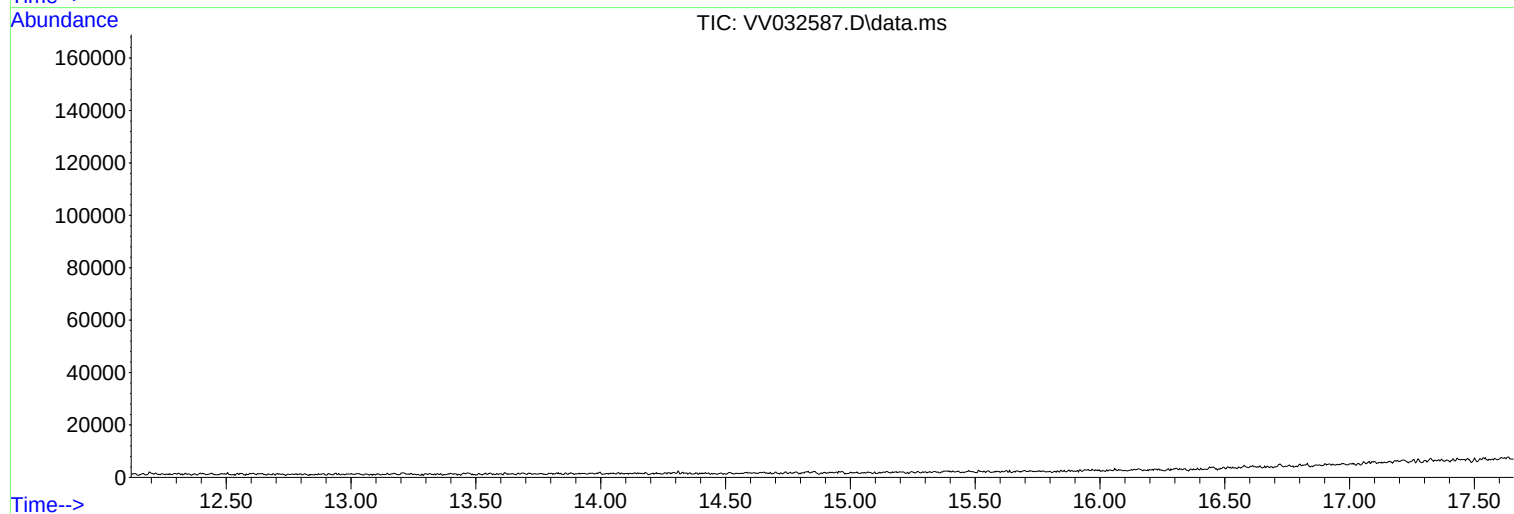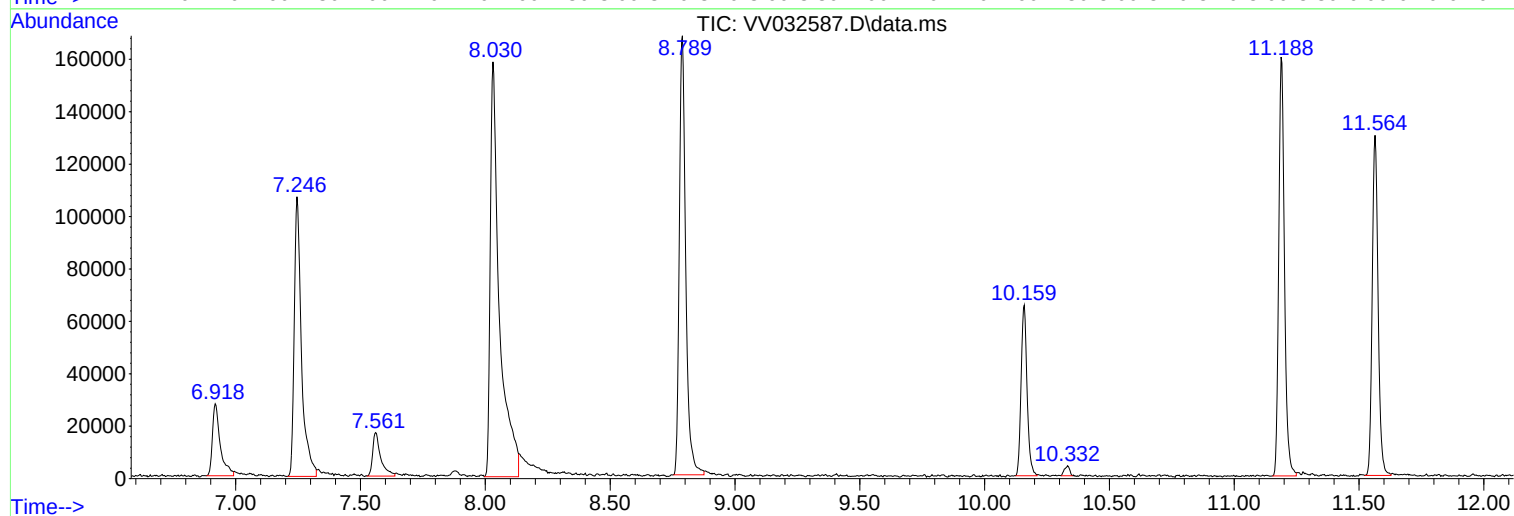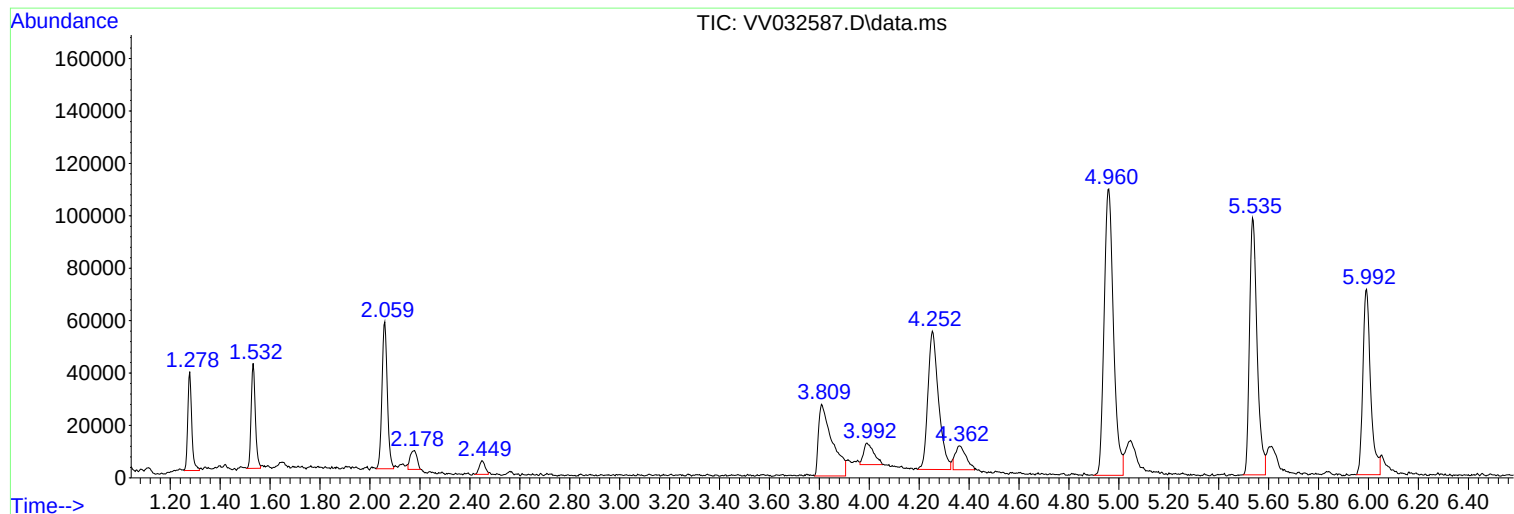

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032587.D
Acq On : 24 Oct 2023 14:03
Operator : SY/MD
Sample : 04962-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COALO










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethyl Acetate Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.992	0.56 ug/L	23417	1,4-Difluorobenzene	5.538

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethyl Acetate	88	C4H8O2	000141-78-6	86
2			Ethyl Acetate	88	C4H8O2	000141-78-6	78
3			Ethyl Acetate	88	C4H8O2	000141-78-6	78
4			Ethyl Acetate	88	C4H8O2	000141-78-6	72
5			CH3C(O)CH2CH2OH	88	C4H8O2	000590-90-9	59

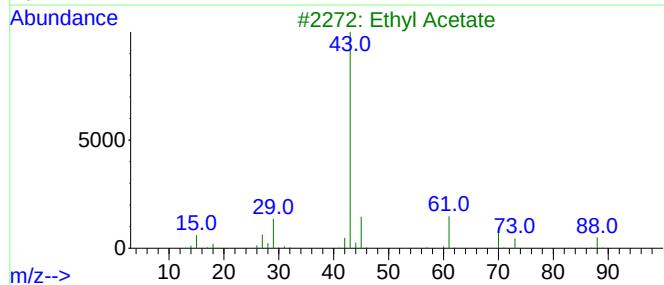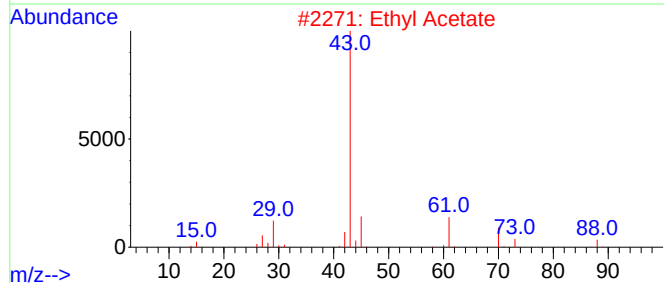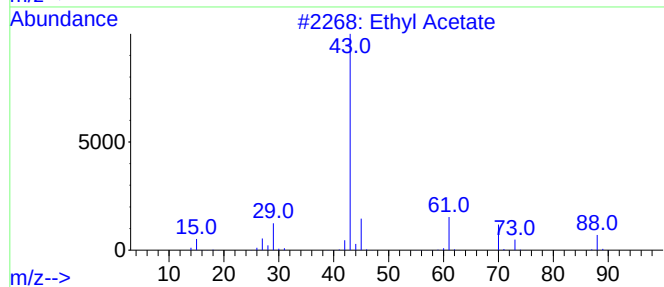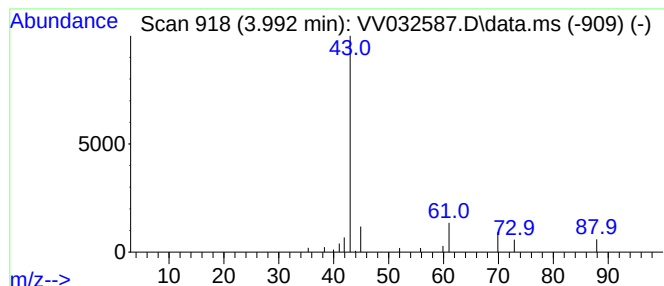

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032587.D
Acq On : 24 Oct 2023 14:03
Operator : SY/MD
Sample : 04962-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethyl Acetate	3.992	0.6	ug/L	23417	1	5.538	208206	5.0