

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
 Data File : VV032594.D
 Acq On : 24 Oct 2023 16:53
 Operator : SY/MD
 Sample : 04993-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	20	25	35	rVB	6297	8606	1.98%	0.290%
2	1.278	68	74	85	rVB	35873	38086	8.74%	1.284%
3	1.388	102	108	113	rBV	3755	4408	1.01%	0.149%
4	1.532	146	153	164	rVB	39979	46321	10.63%	1.562%
5	2.060	305	317	333	rBV	51573	77115	17.70%	2.600%
6	2.188	346	357	367	rBV2	9297	17149	3.94%	0.578%
7	2.314	382	396	398	rBV6	3210	6113	1.40%	0.206%
8	2.619	479	491	492	rBV4	3262	5294	1.22%	0.178%
9	3.809	846	861	892	rBV3	53233	201168	46.18%	6.782%
10	4.252	981	999	1018	rBV2	45068	117733	27.03%	3.969%
11	4.371	1026	1036	1054	rVB2	10369	25134	5.77%	0.847%
12	4.960	1203	1219	1237	rBV2	103600	271260	62.28%	9.145%
13	5.056	1241	1249	1266	rVB7	12089	32252	7.40%	1.087%
14	5.539	1386	1399	1414	rBV	100485	212507	48.79%	7.164%
15	5.612	1416	1422	1441	rVB2	11144	27835	6.39%	0.938%
16	5.992	1525	1540	1554	rBV2	69255	146302	33.59%	4.932%
17	6.918	1816	1828	1843	rBV2	27003	55636	12.77%	1.876%
18	7.246	1920	1930	1955	rBV	102017	205644	47.21%	6.933%
19	7.561	2019	2028	2047	rBV	17341	34820	7.99%	1.174%
20	7.908	2126	2136	2157	rVB	53488	101986	23.41%	3.438%
21	8.030	2162	2174	2209	rBV	205485	435573	100.00%	14.685%
22	8.786	2398	2409	2431	rBV	174369	313728	72.03%	10.577%
23	10.156	2823	2835	2854	rBV	68174	110142	25.29%	3.713%
24	11.188	3145	3156	3173	rBV	163711	260534	59.81%	8.784%
25	11.564	3262	3273	3293	rBV	126725	205015	47.07%	6.912%
26	12.294	3491	3500	3508	rBV8	3681	5761	1.32%	0.194%




Sum of corrected areas: 2966122

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032594.D
Acq On : 24 Oct 2023 16:53
Operator : SY/MD
Sample : 04993-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

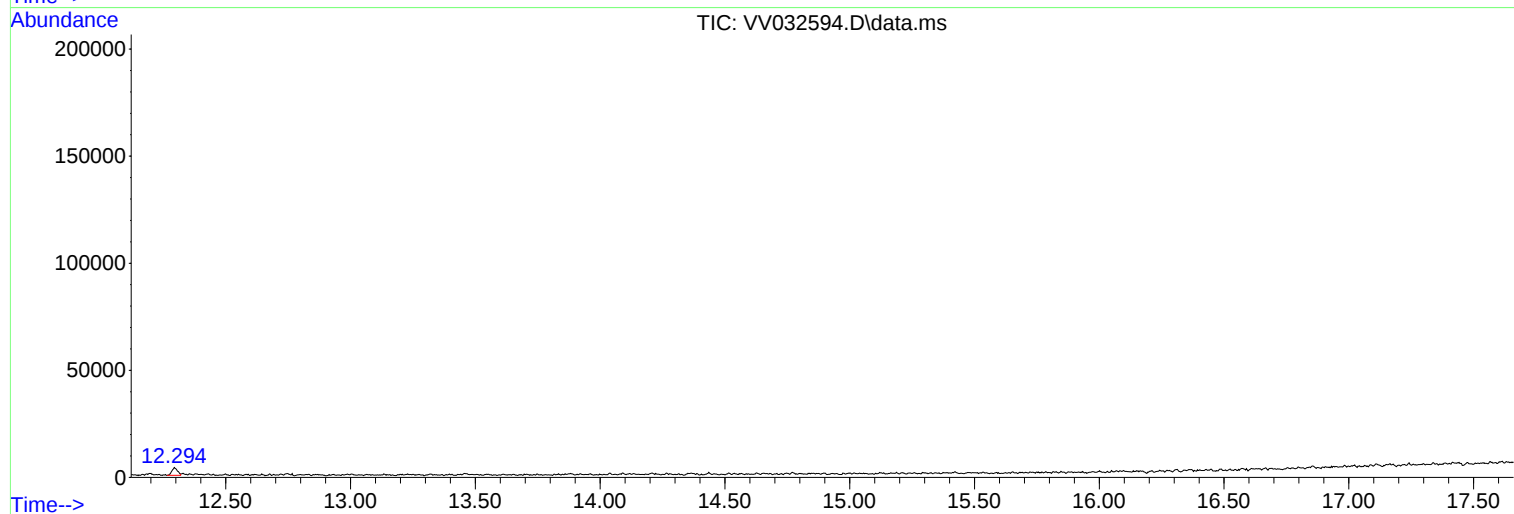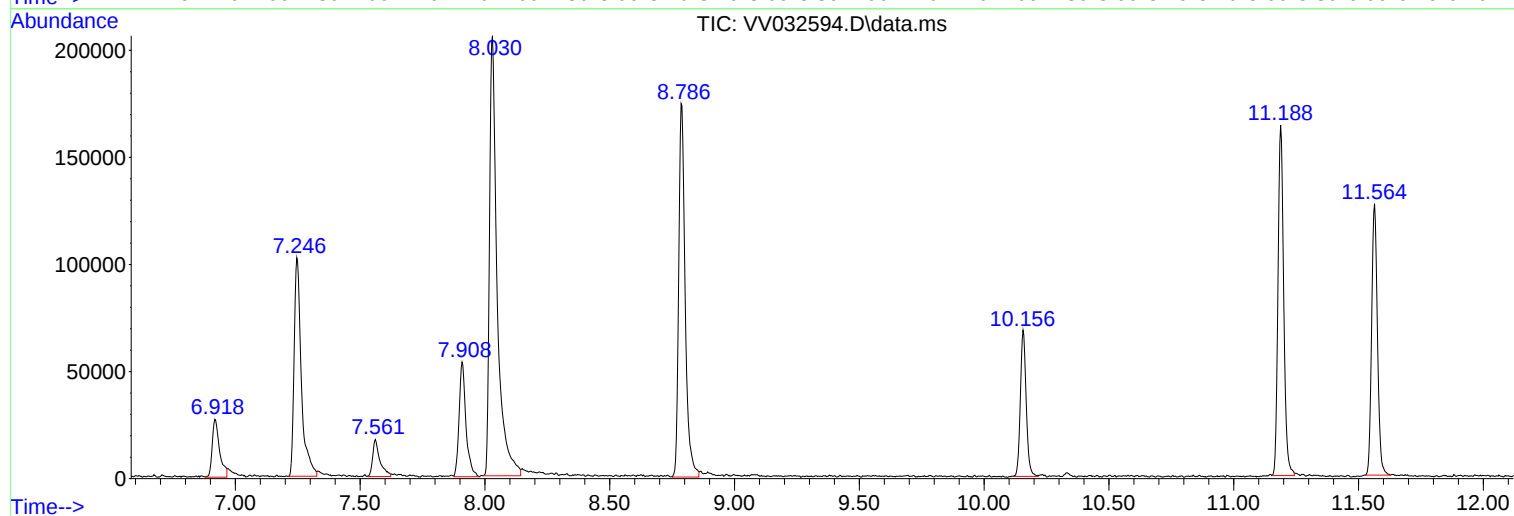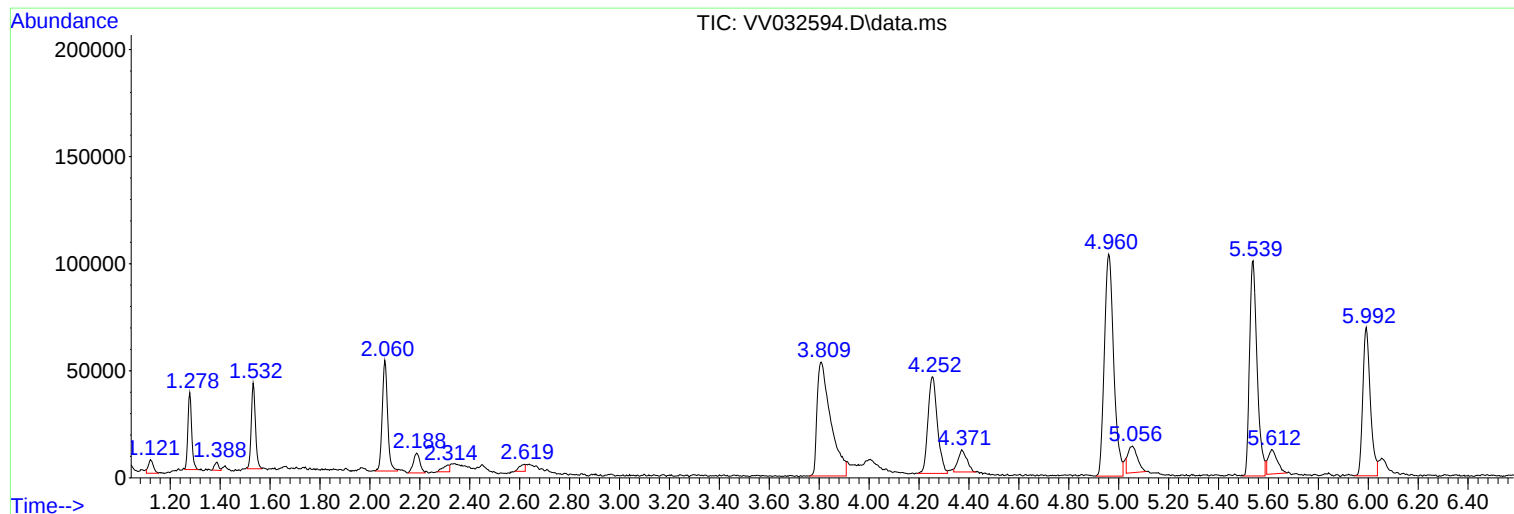

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032594.D
Acq On : 24 Oct 2023 16:53
Operator : SY/MD
Sample : 04993-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032594.D
Acq On : 24 Oct 2023 16:53
Operator : SY/MD
Sample : 04993-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------