

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
 Data File : VV032607.D
 Acq On : 24 Oct 2023 22:33
 Operator : SY/MD
 Sample : VV1024WBL03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK379

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.117	19	24	35	rVB	5047	7528	1.80%	0.230%
2	1.278	67	74	91	rVB	62001	66580	15.93%	2.035%
3	1.532	146	153	167	rBV	56204	66259	15.85%	2.025%
4	2.059	307	317	343	rVB	92364	142555	34.10%	4.357%
5	2.182	343	355	371	rVB2	14820	30198	7.22%	0.923%
6	3.809	852	861	863	rBV	26850	33909	8.11%	1.036%
7	4.252	980	999	1021	rBV	59605	158440	37.90%	4.842%
8	4.365	1021	1034	1051	rVB2	10187	29049	6.95%	0.888%
9	4.960	1200	1219	1238	rBV3	148077	380100	90.92%	11.616%
10	5.053	1239	1248	1271	rVB4	14615	45352	10.85%	1.386%
11	5.538	1384	1399	1415	rBV	106749	228205	54.59%	6.974%
12	5.992	1525	1540	1555	rBV2	88762	187009	44.73%	5.715%
13	6.918	1817	1828	1849	rBV	38961	82252	19.67%	2.514%
14	7.246	1918	1930	1955	rBV	170039	332130	79.45%	10.150%
15	7.561	2018	2028	2049	rBV2	24267	50092	11.98%	1.531%
16	8.030	2164	2174	2222	rBV	161702	418058	100.00%	12.777%
17	8.789	2398	2410	2427	rBV	183093	321806	76.98%	9.835%
18	10.156	2825	2835	2852	rBV	69126	115710	27.68%	3.536%
19	11.188	3145	3156	3176	rBV	177606	285510	68.29%	8.726%
20	11.278	3176	3184	3193	rVB6	5031	7655	1.83%	0.234%
21	11.564	3261	3273	3289	rBV	172368	283680	67.86%	8.670%




Sum of corrected areas: 3272077

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032607.D
Acq On : 24 Oct 2023 22:33
Operator : SY/MD
Sample : VV1024WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK379

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

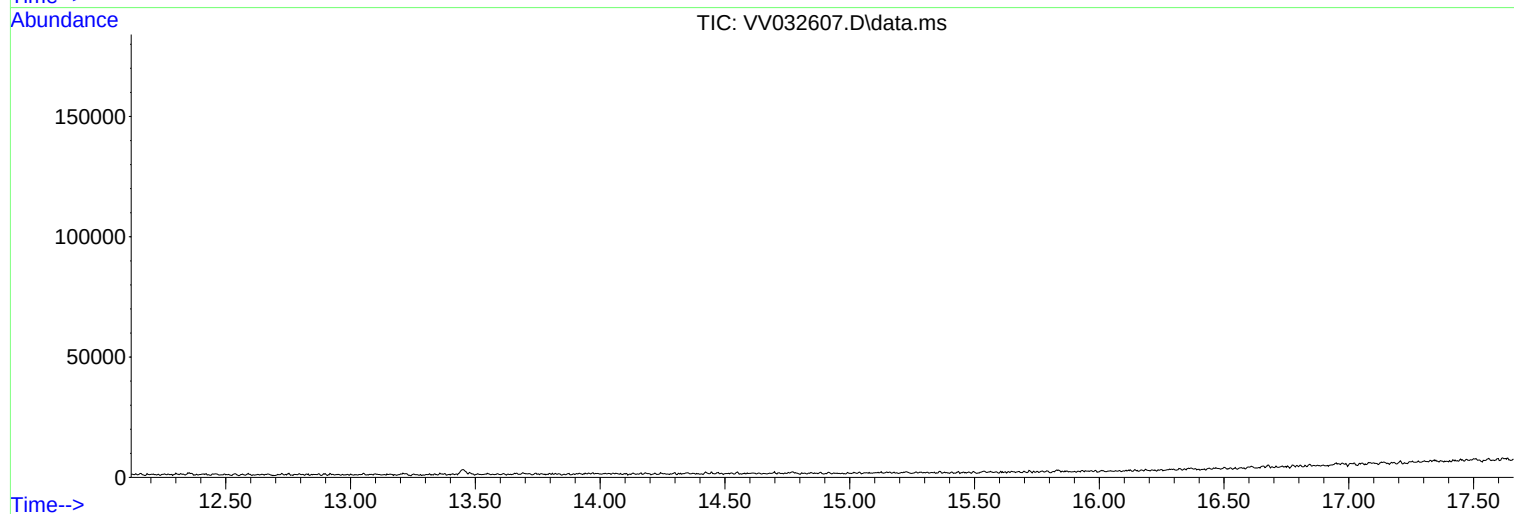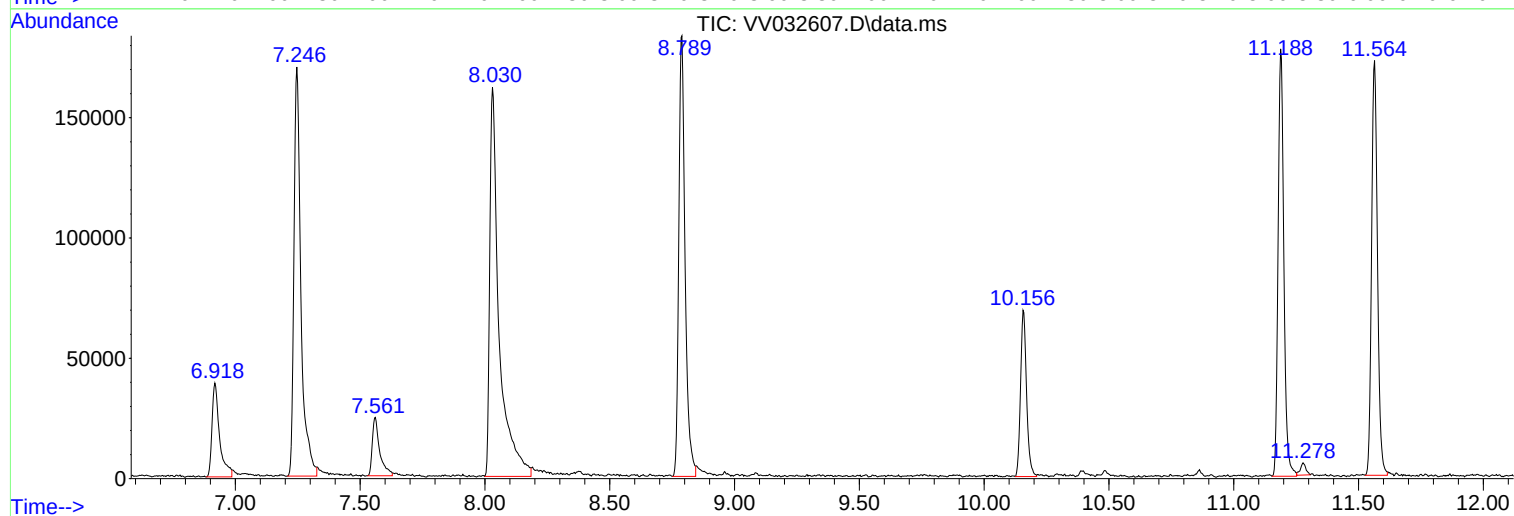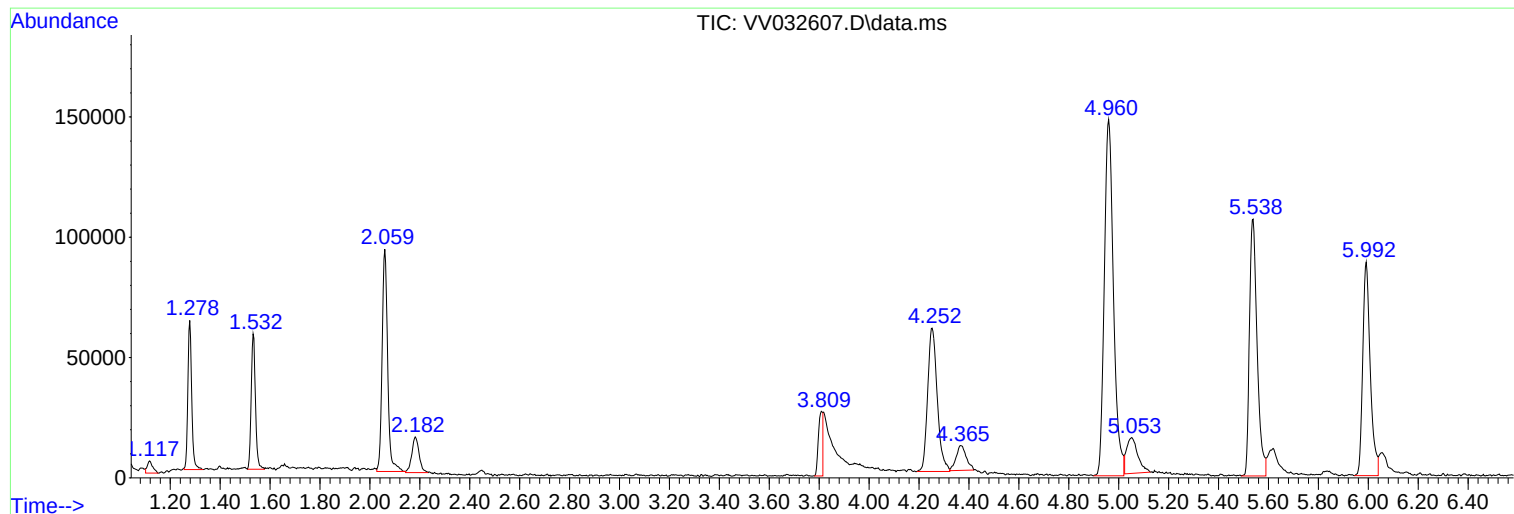

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032607.D
Acq On : 24 Oct 2023 22:33
Operator : SY/MD
Sample : VV1024WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK379

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032607.D
Acq On : 24 Oct 2023 22:33
Operator : SY/MD
Sample : VV1024WBL03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK379

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------