

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
 Data File : VV032612.D
 Acq On : 25 Oct 2023 00:34
 Operator : SY/MD
 Sample : 04995-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4945

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032612.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	20	24	33	rVB	4262	5504	1.19%	0.168%
2	1.217	49	55	62	rBV	8766	10163	2.19%	0.310%
3	1.278	66	74	88	rVV	35152	40029	8.64%	1.221%
4	1.385	101	107	115	rBV	30425	34852	7.53%	1.063%
5	1.532	135	153	164	rBV	44123	60927	13.16%	1.859%
6	2.060	307	317	328	rBV	53283	77193	16.67%	2.355%
7	2.185	346	356	372	rVB2	8459	18298	3.95%	0.558%
8	2.565	463	474	486	rVB10	2523	6240	1.35%	0.190%
9	3.806	842	860	895	rBV3	119856	428375	92.51%	13.069%
10	4.253	983	999	1022	rBV	50562	132454	28.60%	4.041%
11	4.372	1024	1036	1056	rVB3	9274	26122	5.64%	0.797%
12	4.960	1203	1219	1238	rBV2	115198	300495	64.89%	9.167%
13	5.539	1388	1399	1416	rBV	108866	229213	49.50%	6.993%
14	5.992	1522	1540	1554	rBV	75052	158333	34.19%	4.830%
15	6.918	1817	1828	1857	rBV2	31179	67556	14.59%	2.061%
16	7.246	1919	1930	1955	rBV	111832	222621	48.08%	6.792%
17	7.561	2016	2028	2054	rBV	20063	43754	9.45%	1.335%
18	8.027	2164	2173	2206	rBV	224666	463064	100.00%	14.127%
19	8.789	2398	2410	2437	rBV	183502	325580	70.31%	9.933%
20	10.156	2823	2835	2851	rBV	74908	117295	25.33%	3.578%
21	11.188	3142	3156	3172	rBV	179064	284882	61.52%	8.691%
22	11.564	3262	3273	3288	rVB	142430	224927	48.57%	6.862%




Sum of corrected areas: 3277877

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032612.D
Acq On : 25 Oct 2023 00:34
Operator : SY/MD
Sample : 04995-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4945

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

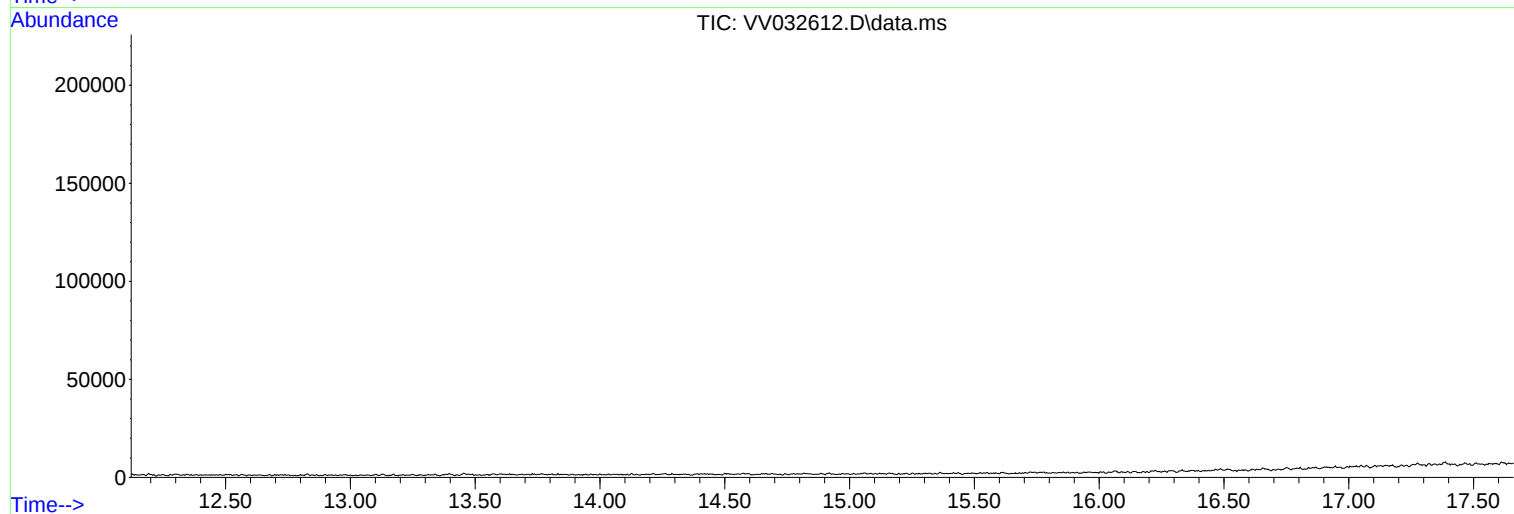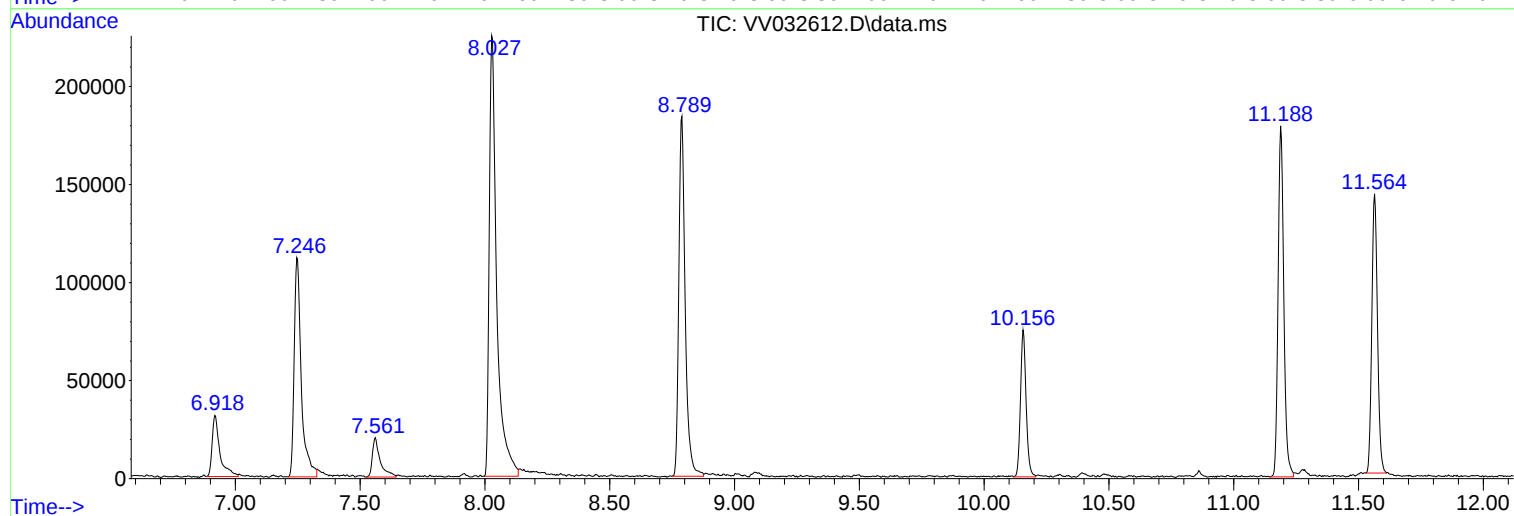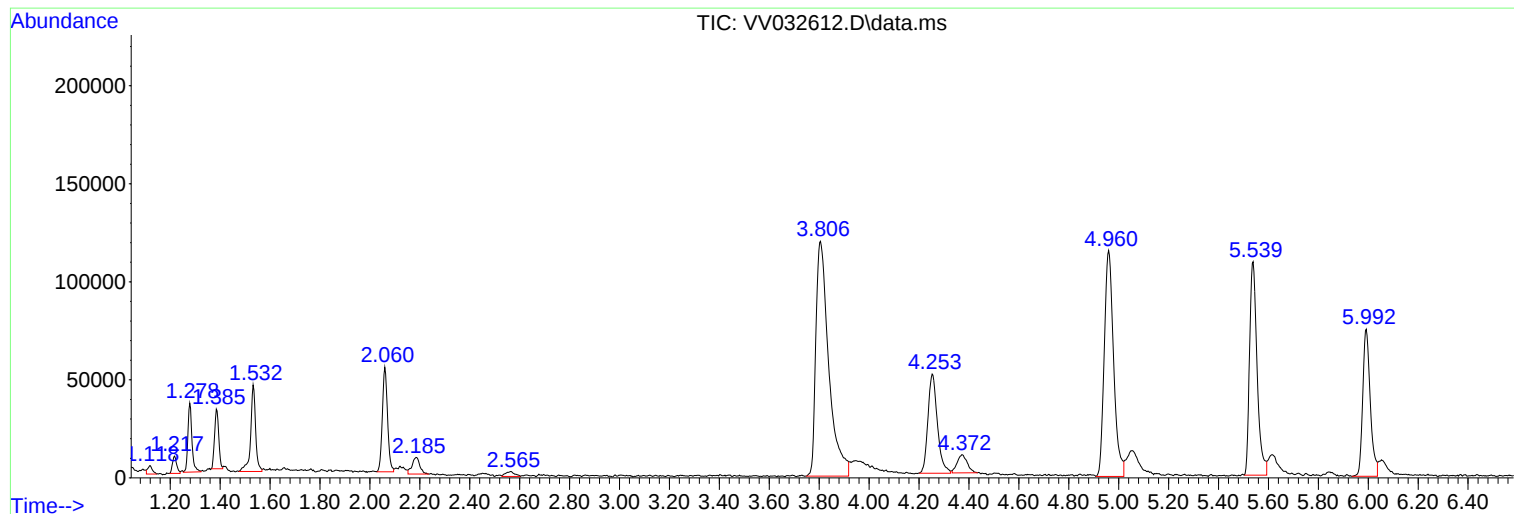

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032612.D
Acq On : 25 Oct 2023 00:34
Operator : SY/MD
Sample : 04995-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4945

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032612.D
Acq On : 25 Oct 2023 00:34
Operator : SY/MD
Sample : 04995-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4945

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------