

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
 Data File : VV032613.D
 Acq On : 25 Oct 2023 00:59
 Operator : SY/MD
 Sample : 04995-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4947

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032613.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	20	24	36	rVB	4669	7000	1.48%	0.233%
2	1.278	65	74	92	rBV	37914	42468	8.95%	1.412%
3	1.532	144	153	166	rVB	43739	51816	10.92%	1.723%
4	2.060	307	317	330	rBV2	53500	78914	16.64%	2.624%
5	2.188	348	357	370	rVB2	10215	18908	3.99%	0.629%
6	3.799	847	858	890	rBV	53836	174004	36.69%	5.786%
7	4.253	983	999	1023	rBV	50900	138690	29.24%	4.612%
8	4.368	1023	1035	1053	rVB3	9907	28929	6.10%	0.962%
9	4.960	1205	1219	1238	rBV2	115101	297573	62.74%	9.896%
10	5.053	1240	1248	1273	rVB5	12607	38357	8.09%	1.276%
11	5.539	1386	1399	1415	rBV	97757	208514	43.96%	6.934%
12	5.616	1417	1423	1441	rVB3	9674	22398	4.72%	0.745%
13	5.992	1527	1540	1554	rBV	77054	159023	33.53%	5.288%
14	6.918	1817	1828	1844	rBV	31559	64932	13.69%	2.159%
15	7.246	1919	1930	1950	rBV	113542	225169	47.47%	7.488%
16	7.561	2019	2028	2044	rBV2	19498	38990	8.22%	1.297%
17	8.027	2161	2173	2206	rBV	230645	474312	100.00%	15.773%
18	8.789	2399	2410	2431	rBV	168140	297021	62.62%	9.877%
19	9.085	2493	2502	2515	rBV5	6050	10873	2.29%	0.362%
20	10.156	2821	2835	2854	rBV	73788	119843	25.27%	3.985%
21	10.860	3047	3054	3064	rVB8	3273	5071	1.07%	0.169%
22	11.188	3145	3156	3175	rBV	165642	264707	55.81%	8.803%
23	11.278	3178	3184	3192	rVB9	3722	5266	1.11%	0.175%
24	11.564	3262	3273	3290	rVB	146153	234346	49.41%	7.793%


Sum of corrected areas: 3007124

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032613.D
Acq On : 25 Oct 2023 00:59
Operator : SY/MD
Sample : 04995-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4947

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

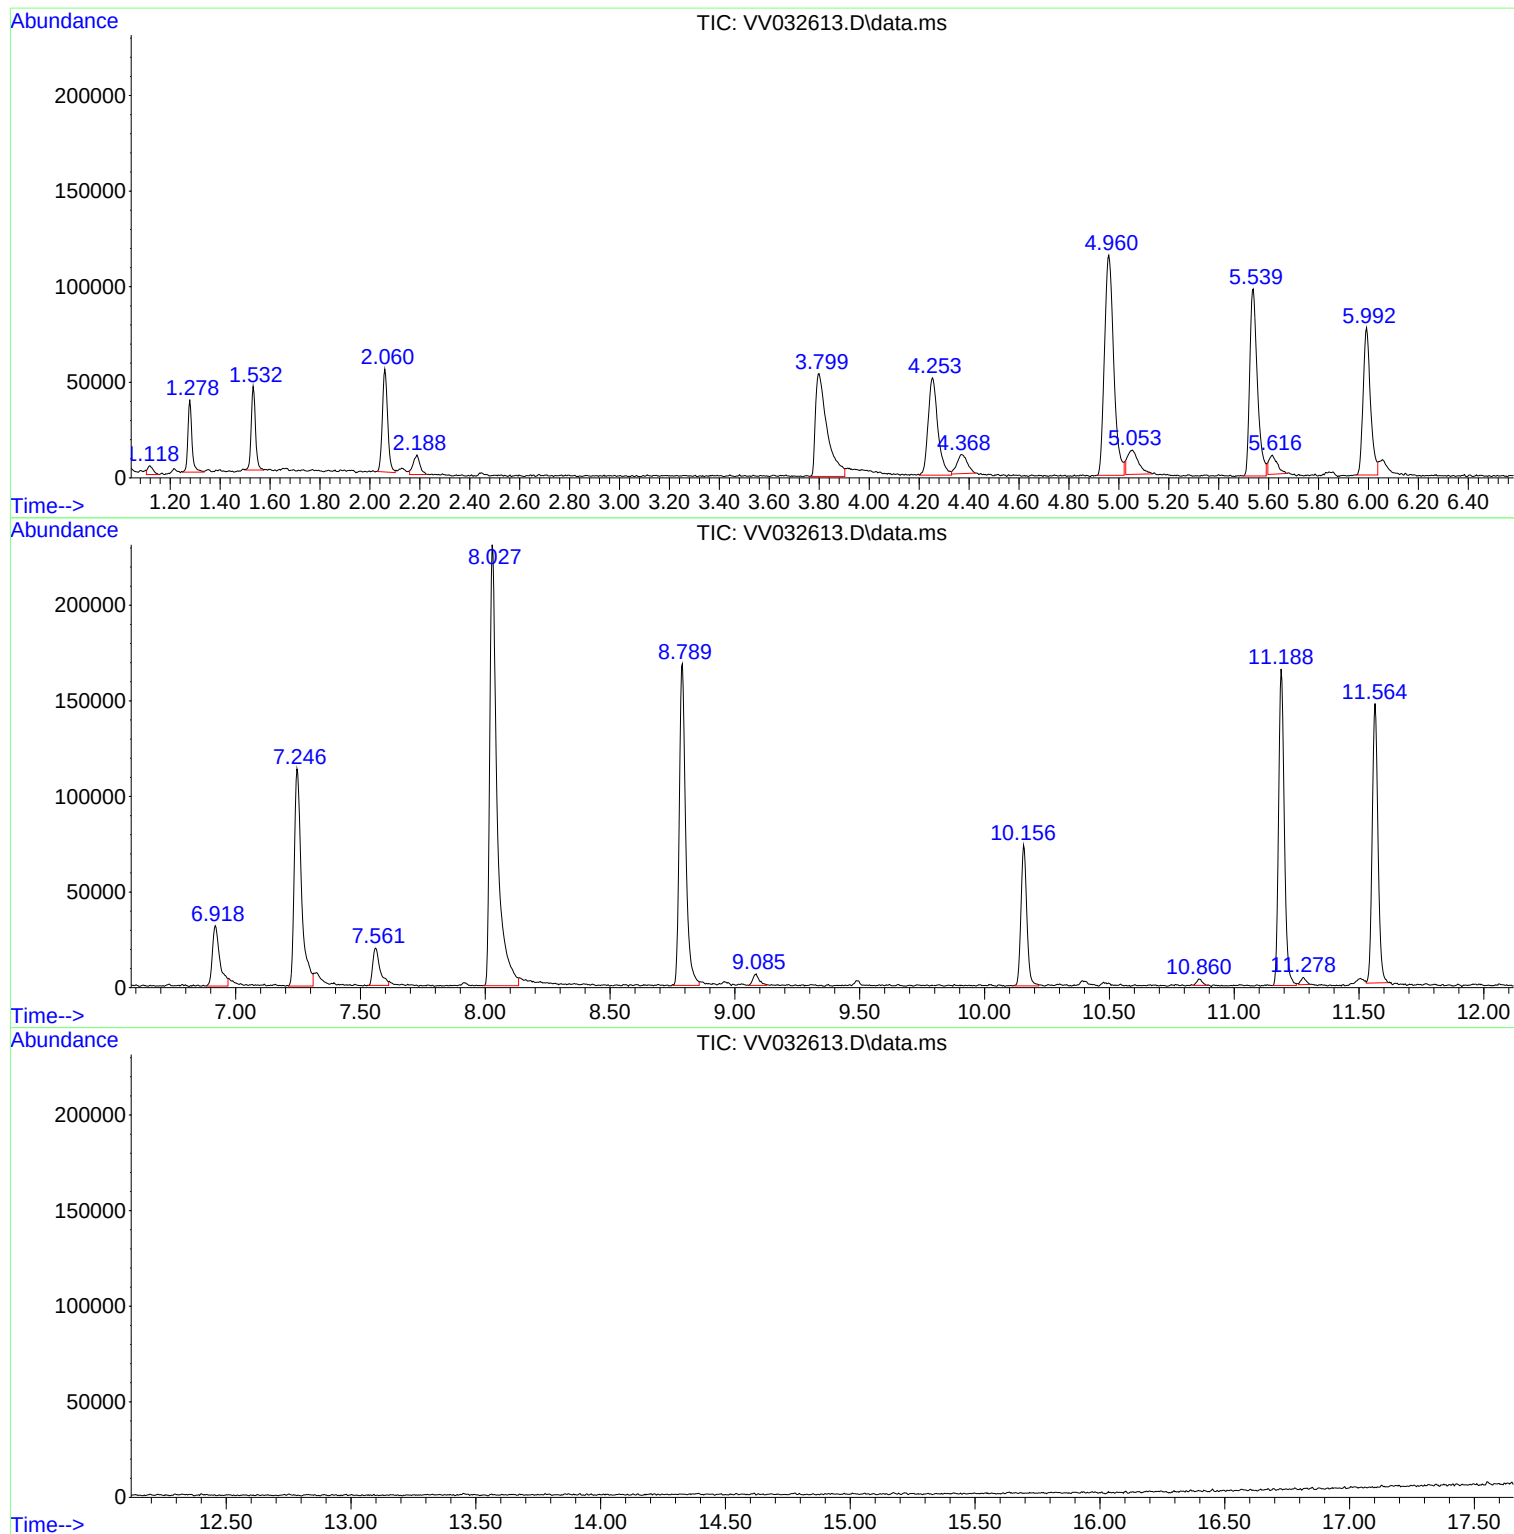

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032613.D
Acq On : 25 Oct 2023 00:59
Operator : SY/MD
Sample : 04995-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4947

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032613.D
Acq On : 25 Oct 2023 00:59
Operator : SY/MD
Sample : 04995-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4947

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
