

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
 Data File : VV032614.D
 Acq On : 25 Oct 2023 01:23
 Operator : SY/MD
 Sample : 04995-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4949

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032614.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.117	20	24	38	rVB	4541	7883	1.81%	0.247%
2	1.278	65	74	85	rBV	33852	39387	9.02%	1.234%
3	1.532	145	153	167	rVB	40667	48660	11.15%	1.525%
4	2.059	306	317	330	rBV	52930	77886	17.84%	2.440%
5	2.182	347	355	368	rVB2	7762	15451	3.54%	0.484%
6	3.799	849	858	887	rBV2	51817	158842	36.39%	4.977%
7	4.256	985	1000	1020	rBV2	48421	129881	29.75%	4.069%
8	4.374	1022	1037	1052	rVB4	8263	23744	5.44%	0.744%
9	4.960	1201	1219	1237	rBV2	107833	282614	64.74%	8.854%
10	5.053	1240	1248	1262	rVB7	9552	26817	6.14%	0.840%
11	5.535	1386	1398	1415	rBV	133395	280937	64.36%	8.802%
12	5.612	1417	1422	1444	rVB3	12820	31622	7.24%	0.991%
13	5.992	1527	1540	1556	rBV	70673	151470	34.70%	4.746%
14	6.918	1817	1828	1854	rBV2	29328	64860	14.86%	2.032%
15	7.246	1918	1930	1950	rBV	107313	215983	49.48%	6.767%
16	7.326	1950	1955	1965	rVB	8682	14654	3.36%	0.459%
17	7.561	2017	2028	2044	rBV	18609	36940	8.46%	1.157%
18	8.030	2163	2174	2202	rBV	208399	436530	100.00%	13.677%
19	8.789	2398	2410	2430	rBV	227039	398789	91.35%	12.494%
20	8.956	2455	2462	2471	rBV4	3013	4972	1.14%	0.156%
21	9.078	2489	2500	2512	rBV3	10105	18555	4.25%	0.581%
22	9.487	2620	2627	2638	rVB5	4438	7664	1.76%	0.240%
23	10.156	2823	2835	2849	rBV	70116	111950	25.65%	3.507%
24	10.394	2901	2909	2914	rBV6	4540	6527	1.50%	0.204%
25	10.860	3047	3054	3066	rVB5	6659	10272	2.35%	0.322%
26	11.188	3146	3156	3174	rBV	223452	351931	80.62%	11.026%
27	11.278	3177	3184	3192	rVB9	4338	7040	1.61%	0.221%
28	11.503	3238	3254	3257	rBV7	5031	10516	2.41%	0.329%
29	11.564	3263	3273	3288	rBV	140932	219432	50.27%	6.875%




Sum of corrected areas: 3191809

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032614.D
Acq On : 25 Oct 2023 01:23
Operator : SY/MD
Sample : 04995-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4949

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

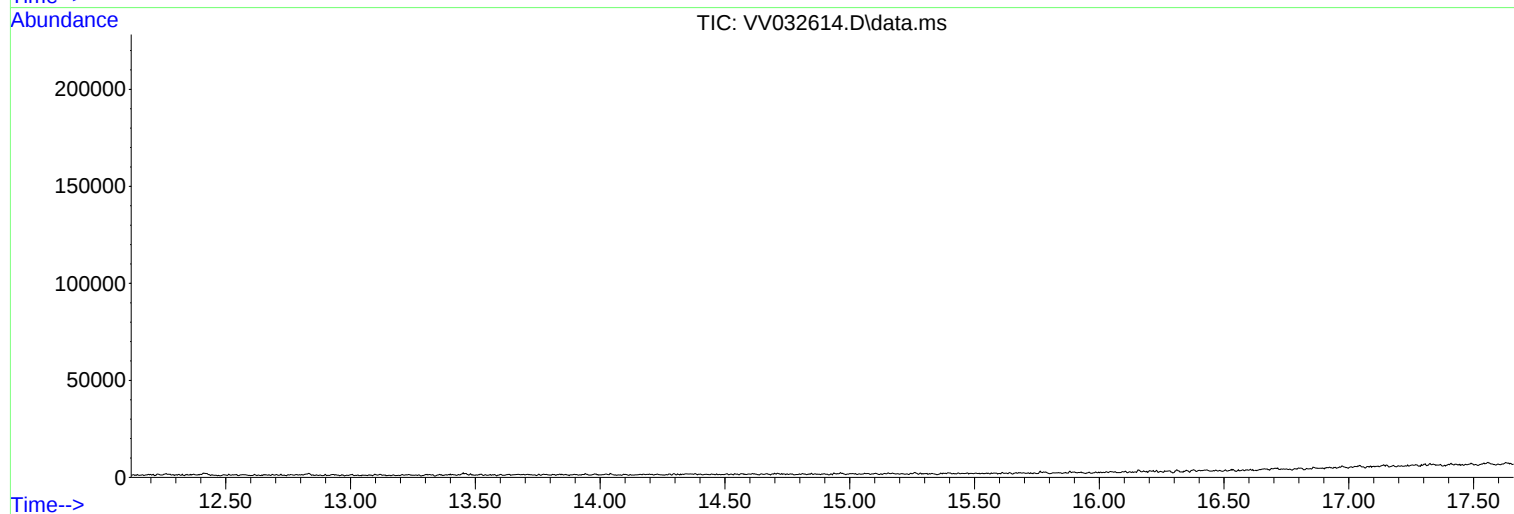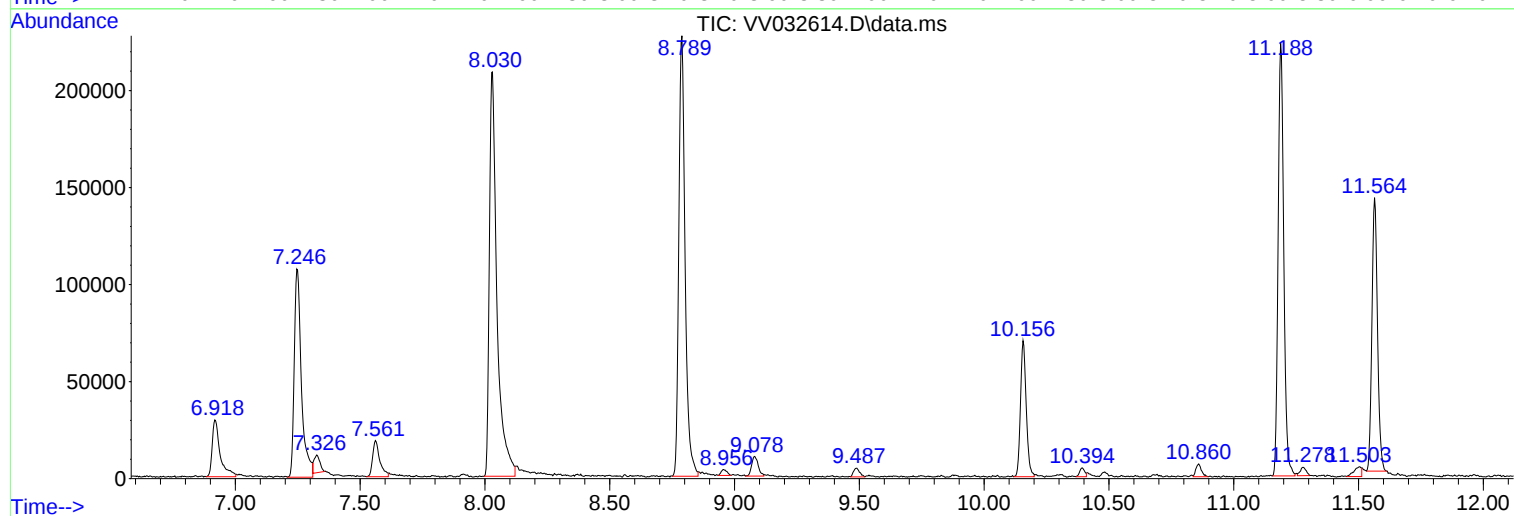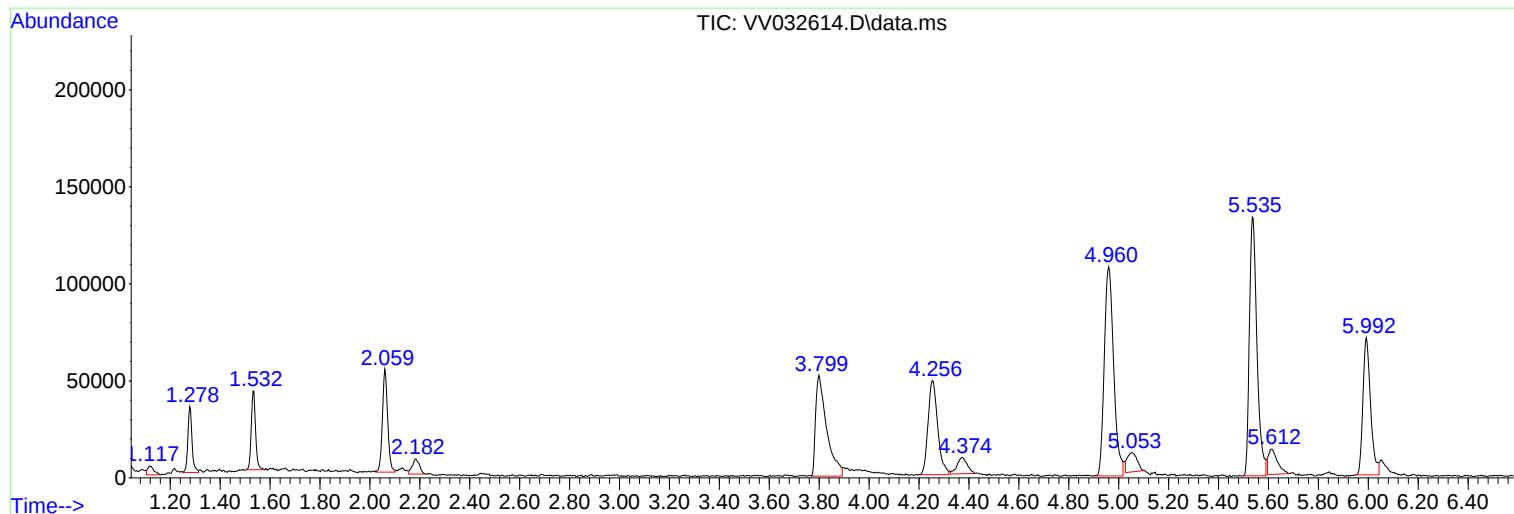

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032614.D
Acq On : 25 Oct 2023 01:23
Operator : SY/MD
Sample : 04995-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4949

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032614.D
Acq On : 25 Oct 2023 01:23
Operator : SY/MD
Sample : 04995-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4949

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------