

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
 Data File : VV032615.D
 Acq On : 25 Oct 2023 01:47
 Operator : SY/MD
 Sample : 04995-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49C3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	86	rBV	34500	37192	8.64%	1.312%
2	1.532	146	153	166	rVB	40595	47989	11.15%	1.693%
3	2.060	308	317	330	rBV	48605	69486	16.14%	2.452%
4	2.185	347	356	367	rVB4	7755	14697	3.41%	0.519%
5	3.799	847	858	884	rBV	49126	155586	36.14%	5.490%
6	4.253	982	999	1020	rBV2	46908	127393	29.59%	4.495%
7	4.375	1022	1037	1056	rVB3	8811	27945	6.49%	0.986%
8	4.960	1202	1219	1239	rBV2	107350	282112	65.52%	9.955%
9	5.053	1239	1248	1262	rVB5	9591	25347	5.89%	0.894%
10	5.539	1387	1399	1415	rBV	101191	211514	49.13%	7.464%
11	5.616	1416	1423	1437	rVB3	9102	20401	4.74%	0.720%
12	5.992	1528	1540	1554	rBV2	69047	150947	35.06%	5.326%
13	6.918	1819	1828	1858	rBV	29203	65973	15.32%	2.328%
14	7.246	1917	1930	1952	rBV	106856	210476	48.88%	7.427%
15	7.561	2019	2028	2056	rBV2	17883	39401	9.15%	1.390%
16	8.031	2163	2174	2206	rBV	202418	430561	100.00%	15.193%
17	8.789	2400	2410	2437	rBV	169931	302242	70.20%	10.665%
18	10.156	2824	2835	2850	rBV	68772	111557	25.91%	3.937%
19	11.188	3146	3156	3176	rBV	167847	266543	61.91%	9.406%
20	11.281	3179	3185	3193	rVB8	2930	4686	1.09%	0.165%
21	11.497	3244	3252	3263	rBV9	5237	12197	2.83%	0.430%
22	11.564	3263	3273	3290	rVB	135338	219659	51.02%	7.751%




Sum of corrected areas: 2833904

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032615.D
Acq On : 25 Oct 2023 01:47
Operator : SY/MD
Sample : 04995-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

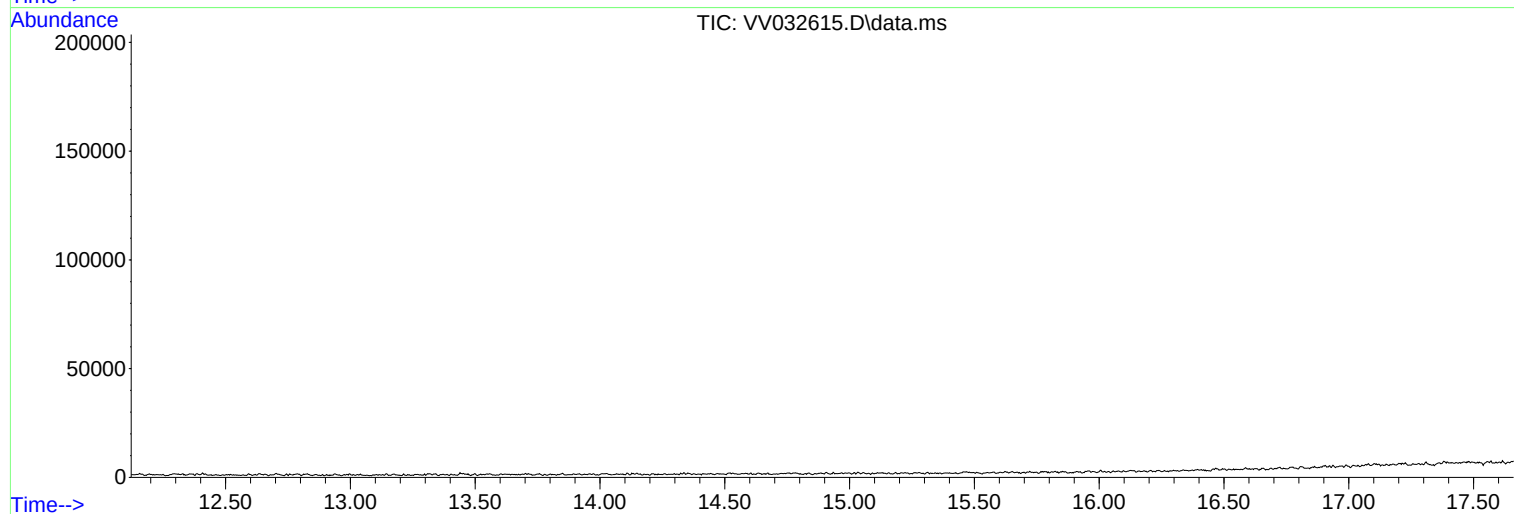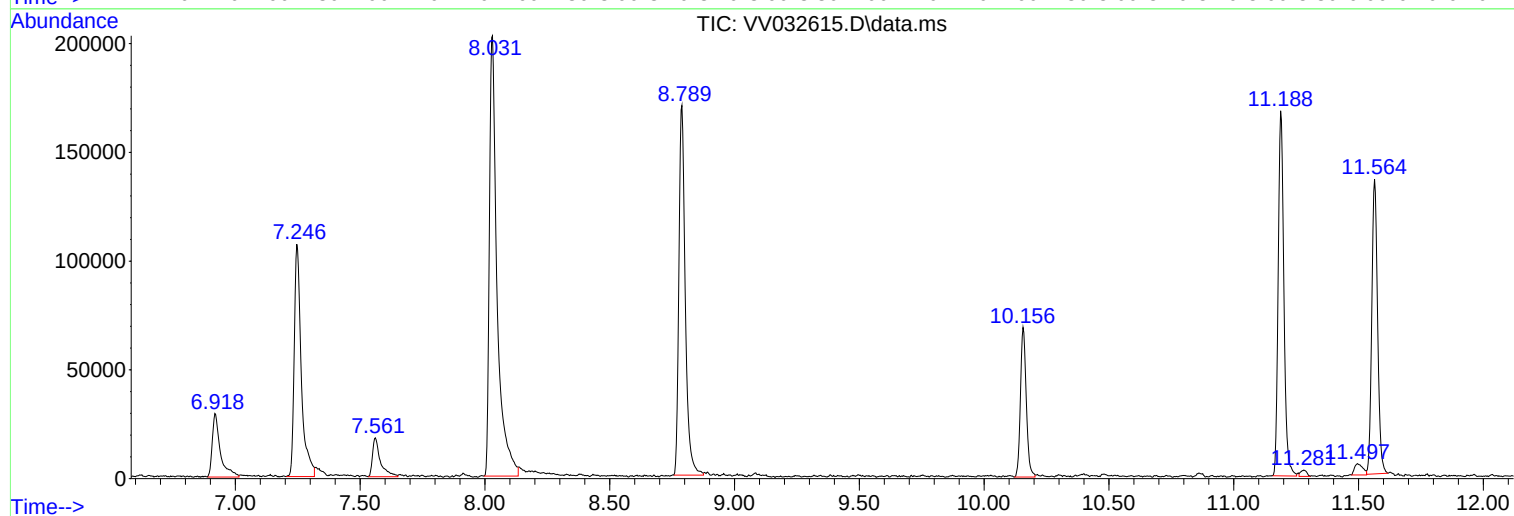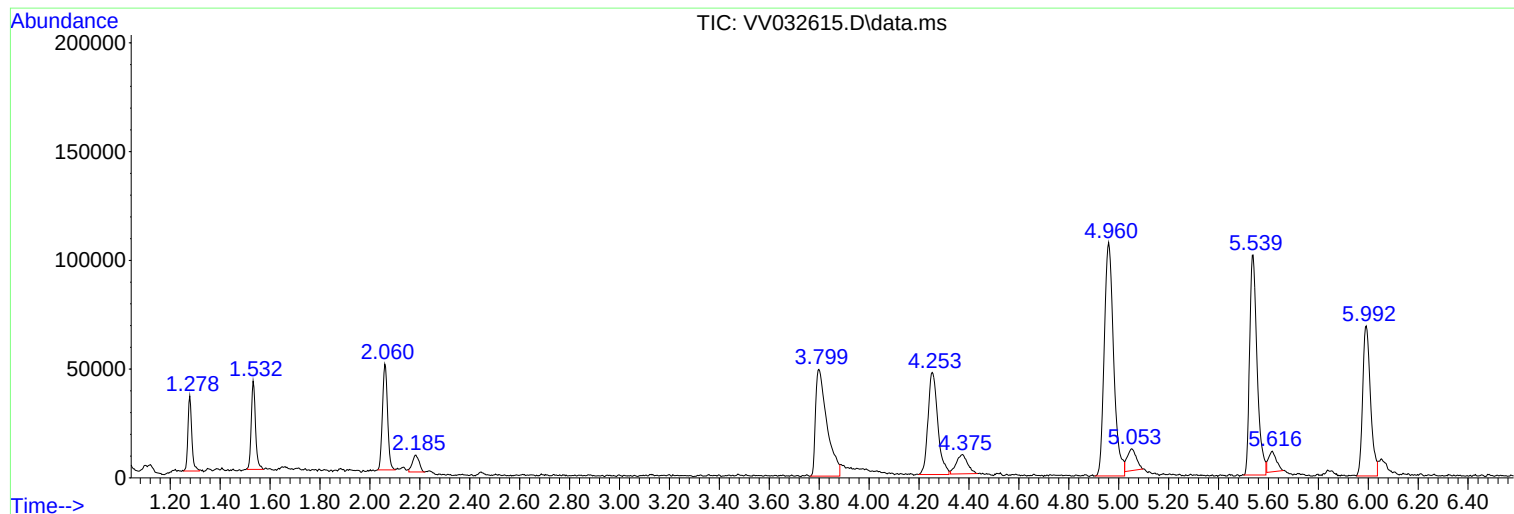

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032615.D
Acq On : 25 Oct 2023 01:47
Operator : SY/MD
Sample : 04995-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032615.D
Acq On : 25 Oct 2023 01:47
Operator : SY/MD
Sample : 04995-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49C3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc