

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
 Data File : VV032618.D
 Acq On : 25 Oct 2023 03:00
 Operator : SY/MD
 Sample : VIBLK326
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK326

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032618.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	18	24	38	rVB	5760	8794	2.60%	0.346%
2	1.278	68	74	87	rVB	29133	31420	9.29%	1.238%
3	1.532	146	153	163	rBV	30011	34345	10.15%	1.353%
4	2.060	308	317	332	rBV	47768	70234	20.76%	2.766%
5	2.182	347	355	368	rVB	8062	15667	4.63%	0.617%
6	2.449	426	438	451	rBV3	11310	19803	5.85%	0.780%
7	3.809	848	861	893	rBV3	35139	133239	39.39%	5.248%
8	4.256	983	1000	1021	rBV	37972	102596	30.33%	4.041%
9	4.371	1025	1036	1037	rBV4	4871	7422	2.19%	0.292%
10	4.960	1204	1219	1239	rBV3	86562	223402	66.05%	8.800%
11	5.053	1242	1248	1261	rVB7	6142	14448	4.27%	0.569%
12	5.535	1386	1398	1415	rBV	113356	237613	70.25%	9.359%
13	5.992	1528	1540	1555	rBV2	55699	119187	35.24%	4.695%
14	6.918	1818	1828	1843	rBV2	23128	46851	13.85%	1.845%
15	7.246	1919	1930	1961	rBV	93035	183391	54.22%	7.224%
16	7.564	2018	2029	2042	rBV4	13934	28282	8.36%	1.114%
17	8.030	2165	2174	2209	rBV	119412	273251	80.79%	10.763%
18	8.368	2270	2279	2292	rVB4	6032	10516	3.11%	0.414%
19	8.786	2398	2409	2435	rBV	186949	338235	100.00%	13.323%
20	10.156	2824	2835	2851	rBV	52047	86228	25.49%	3.396%
21	10.863	3044	3055	3070	rBV7	3295	5451	1.61%	0.215%
22	11.127	3129	3137	3146	rBV7	3120	5361	1.58%	0.211%
23	11.188	3146	3156	3177	rVV	186473	298701	88.31%	11.766%
24	11.564	3262	3273	3293	rVB	123101	199015	58.84%	7.839%
25	12.587	3585	3591	3598	rBV6	4174	6105	1.80%	0.240%
26	13.207	3775	3784	3797	rVB6	6968	10492	3.10%	0.413%
27	13.442	3847	3857	3869	rBV	9645	17833	5.27%	0.702%
28	13.686	3924	3933	3942	rVB8	6968	10875	3.22%	0.428%




Sum of corrected areas: 2538757

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032618.D
Acq On : 25 Oct 2023 03:00
Operator : SY/MD
Sample : VIBLK326
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

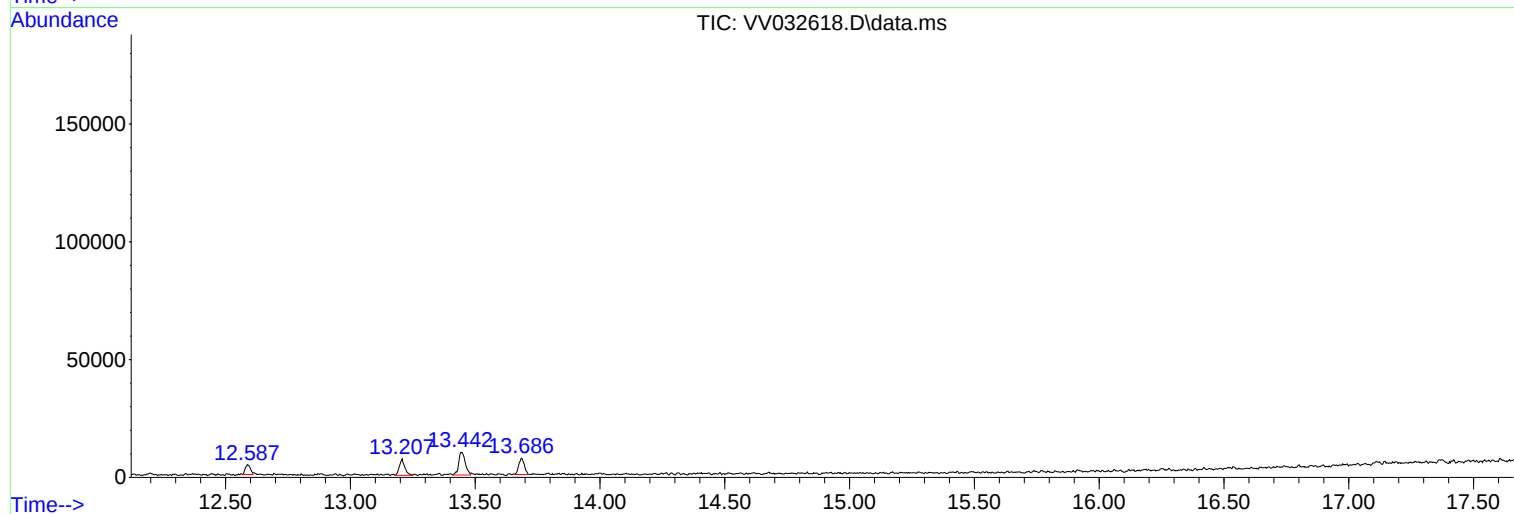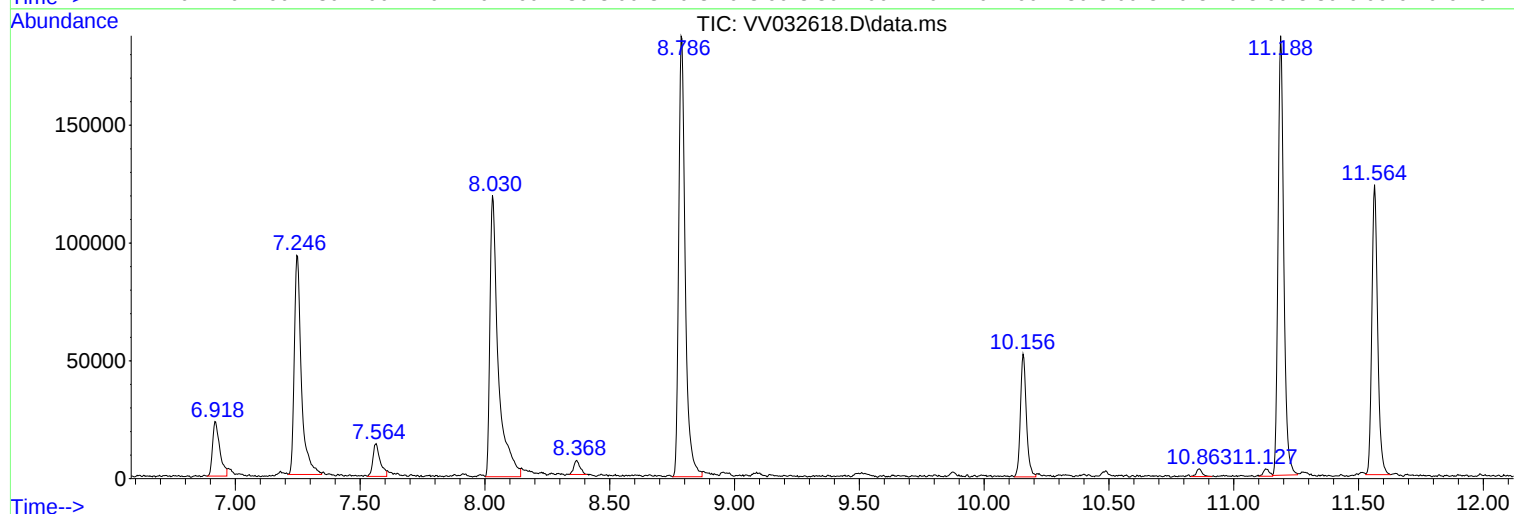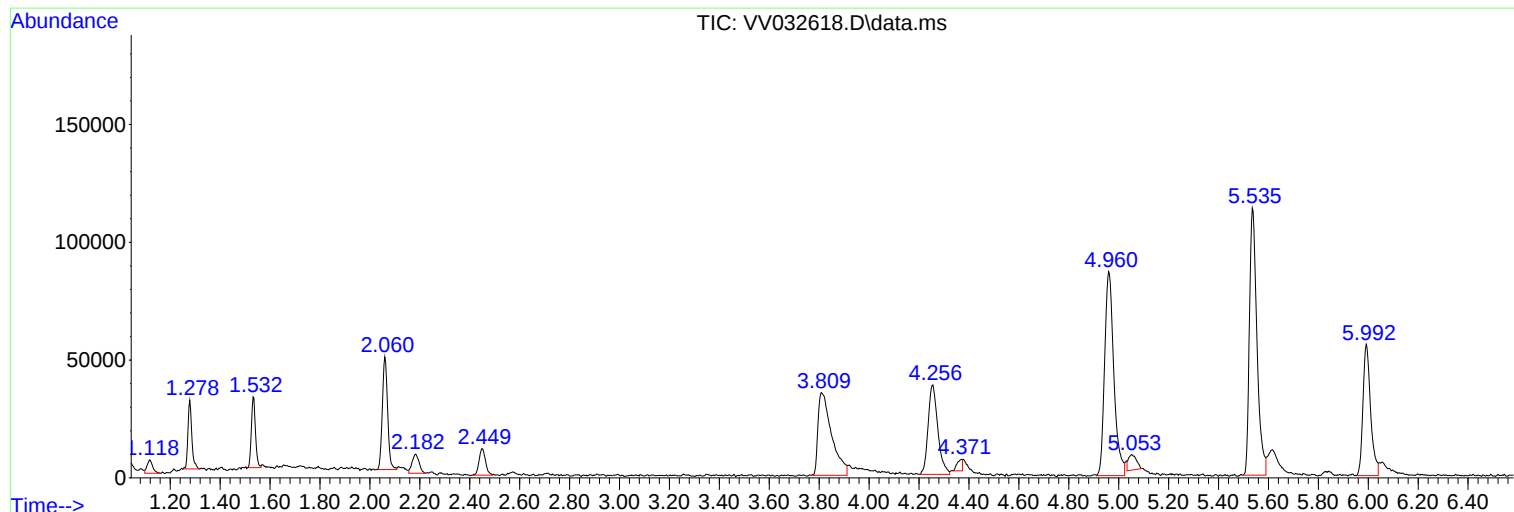

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032618.D
Acq On : 25 Oct 2023 03:00
Operator : SY/MD
Sample : VIBLK326
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032618.D
Acq On : 25 Oct 2023 03:00
Operator : SY/MD
Sample : VIBLK326
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------