
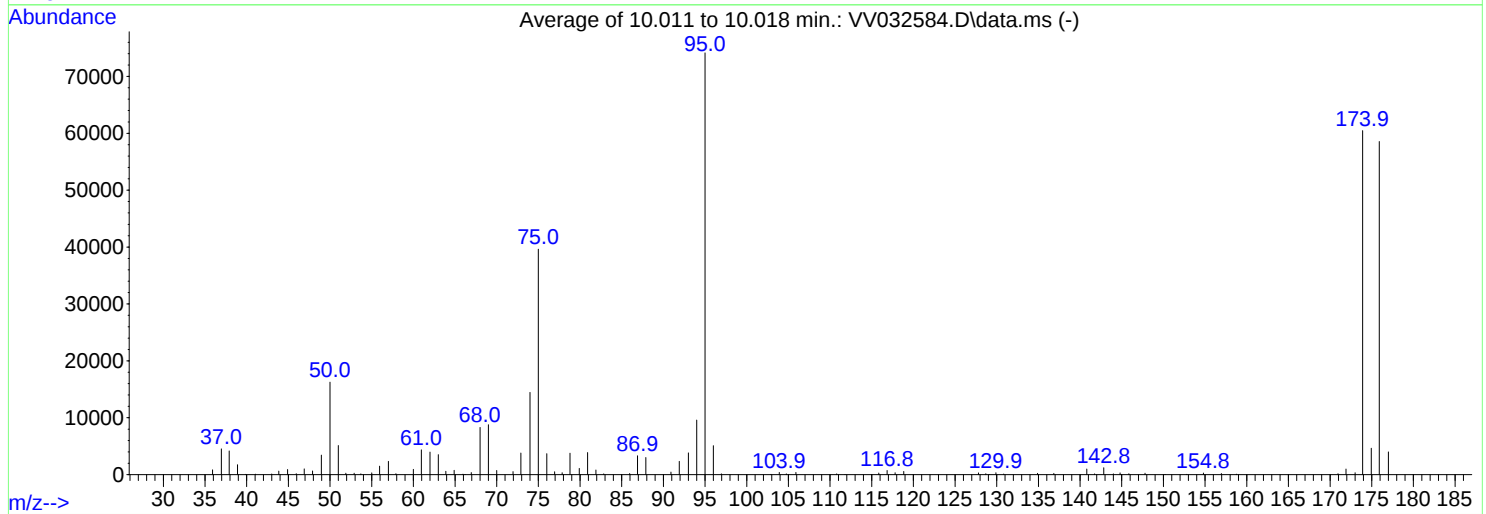


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102423\
Data File : VV032584.D
Acq On : 24 Oct 2023 09:44
Operator : SY/MD
Sample : BFB226
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB226

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Oct 27 05:30:38 2023

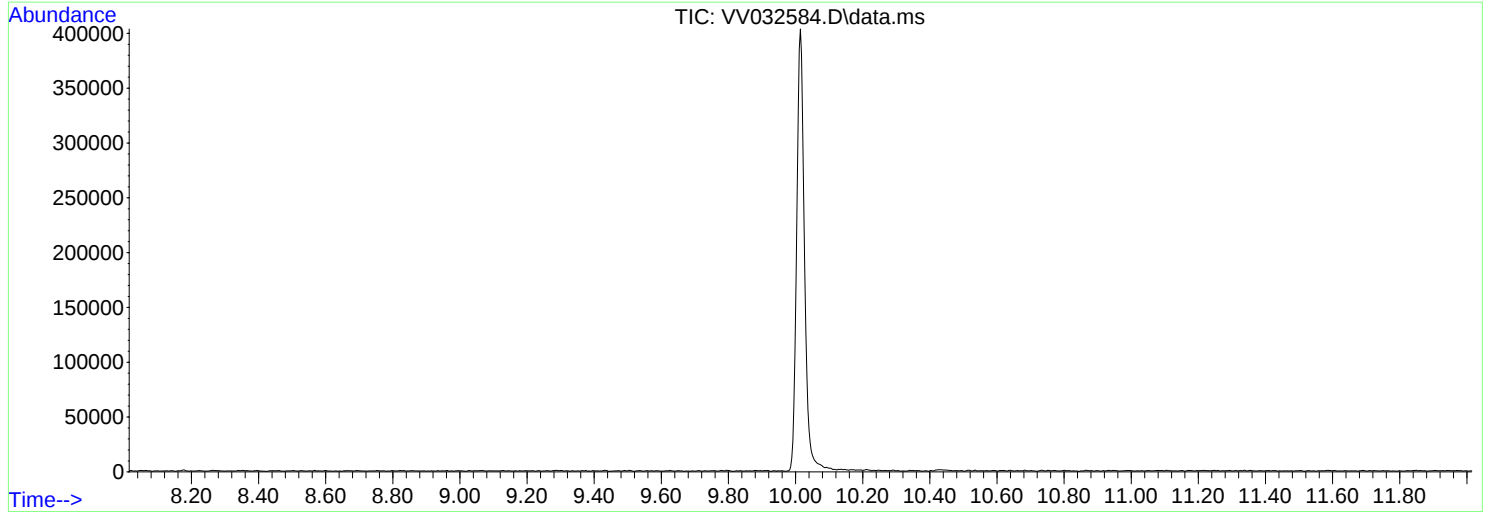

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.9	16249	PASS
75	95	30	80	53.5	39643	PASS
95	95	100	100	100.0	74141	PASS
96	95	5	9	6.9	5107	PASS
173	174	0.00	2	0.6	342	PASS
174	95	50	120	81.6	60480	PASS
175	174	5	9	7.7	4647	PASS
176	174	95	105	96.8	58555	PASS
177	176	5	10	6.8	4007	PASS

m/z	Abundance
37.90	103.0
40.00	233.0
43.80	212.0
50.20	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
35.90	780.0
36.90	4523.0
38.00	4371.0
38.90	1799.0
39.90	279.0
43.00	123.0
43.90	846.0
44.90	877.0
45.90	146.0
46.90	969.0
47.90	660.0
48.90	3424.0
50.00	16528.0
51.00	5205.0
51.90	293.0
52.90	232.0
53.70	131.0
55.00	277.0
55.90	1550.0
57.00	2440.0
57.90	161.0
60.00	903.0
60.90	4198.0
62.00	4126.0
63.00	3523.0
63.90	559.0
64.90	786.0
65.90	151.0
67.00	334.0
68.00	8454.0
69.00	8805.0
70.00	784.0
72.00	505.0
72.90	3871.0
74.00	14423.0
75.00	39456.0
76.00	3640.0
77.00	520.0
77.80	280.0
78.80	3793.0
79.90	966.0
80.90	3800.0
81.90	849.0
82.90	136.0
86.00	195.0
86.90	3360.0
87.90	3037.0
90.90	429.0
91.90	2389.0
93.00	3742.0
94.00	9486.0
95.00	73936.0
96.00	5029.0
96.90	138.0
102.90	106.0
103.90	408.0
104.80	113.0
105.90	380.0
110.80	144.0
115.00	102.0
115.90	310.0
116.90	714.0
117.70	342.0
118.80	575.0
127.80	333.0
128.60	139.0
129.10	103.0
129.90	343.0
130.90	140.0
134.90	229.0
136.90	225.0
140.80	1009.0
141.70	121.0
142.90	1160.0
144.00	139.0
144.80	392.0
145.80	178.0
147.80	243.0
150.20	101.0
154.80	331.0
157.00	195.0
171.00	162.0
171.90	965.0
173.90	58888.0
174.90	4650.0
175.90	56552.0
177.00	3966.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
35.90	870.0
37.00	4688.0
38.00	4426.0
38.90	1793.0
39.80	281.0
41.10	125.0
43.00	118.0
43.90	848.0
44.90	974.0
46.00	163.0
46.90	1055.0
47.90	674.0
49.00	3521.0
50.00	16888.0
51.00	5304.0
51.90	260.0
52.90	282.0
53.70	140.0
55.00	335.0
55.90	1543.0
57.00	2429.0
57.90	174.0
60.00	964.0
61.00	4456.0
62.00	4060.0
63.00	3646.0
63.90	615.0
64.90	775.0
66.00	129.0
66.90	380.0
68.00	8587.0
69.00	9042.0
70.00	738.0
72.00	539.0
72.90	3950.0
74.00	15028.0
75.00	41000.0
76.00	3793.0
77.00	540.0
77.90	349.0
78.80	3894.0
79.90	1126.0
80.90	4021.0
81.90	845.0
82.80	144.0
86.00	200.0
86.90	3386.0
87.90	3137.0
90.90	476.0
91.90	2403.0
93.00	3952.0
94.00	9988.0
95.00	76592.0
96.00	5237.0
97.00	144.0
102.90	102.0
103.90	420.0
104.70	142.0
105.90	386.0
110.80	148.0
115.90	296.0
116.80	723.0
117.80	338.0
118.90	577.0
127.80	336.0
128.70	171.0
129.90	347.0
130.80	125.0
134.90	235.0
136.90	231.0
140.80	1025.0
141.70	148.0
142.90	1277.0
144.00	138.0
144.80	326.0
145.80	178.0
147.80	262.0
152.80	105.0
154.80	310.0
156.90	205.0
158.70	115.0
171.00	149.0
171.90	1014.0
173.00	1027.0
173.90	62456.0
174.90	4805.0
175.90	60696.0
177.00	4144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
35.90	890.0
37.00	4404.0
37.90	4002.0
38.90	1609.0
39.80	296.0
41.00	137.0
43.00	121.0
43.90	806.0
44.90	859.0
46.00	159.0
46.90	1007.0
47.90	635.0
49.00	3347.0
50.00	15640.0
51.00	4884.0
51.90	221.0
52.90	270.0
53.70	129.0
55.00	341.0
56.00	1385.0
57.00	2138.0
57.90	184.0
60.00	912.0
61.00	4412.0
62.00	3729.0
63.00	3364.0
63.90	577.0
64.90	710.0
66.20	119.0
66.90	362.0
68.00	7884.0
69.00	8477.0
70.00	668.0
71.90	532.0
72.90	3584.0
74.00	13891.0
75.00	38472.0
76.00	3603.0
76.90	496.0
77.90	385.0
78.80	3583.0
79.90	1159.0
80.90	3798.0
81.90	782.0
82.80	161.0
85.90	206.0
86.90	3205.0
87.90	2859.0
90.90	435.0
91.90	2219.0
93.00	3824.0
94.00	9314.0
95.00	71896.0
96.00	5054.0
97.00	138.0
103.90	356.0
104.70	183.0
105.90	418.0
110.80	146.0
111.80	108.0
115.80	292.0
116.80	735.0
117.90	321.0
118.90	515.0
127.80	303.0
128.80	181.0
129.90	316.0
130.80	103.0
134.90	203.0
136.80	202.0
140.80	934.0
141.80	161.0
142.80	1231.0
144.00	125.0
144.80	229.0
145.90	176.0
147.80	236.0
152.80	108.0
154.80	254.0
156.90	188.0
158.80	119.0
170.80	171.0
171.90	961.0
173.90	60096.0
175.00	4485.0
175.90	58416.0
177.00	3910.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226