

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102518\
 Data File : VV008415.D
 Acq On : 25 Oct 2018 17:54
 Operator : SY/MD
 Sample : J5635-20
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A40C0

Quant Time: Oct 26 00:13:39 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 25 23:17:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	204231	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	182206	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	72277	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	56675	50.12	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	100.24%
7) Chloroethane-d5	1.57	69	41429	50.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	101.48%
11) 1,1-Dichloroethene-d2	2.13	63	74268	36.36	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.72%
21) 2-Butanone-d5	3.93	46	107698	87.64	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.64%
24) Chloroform-d	4.41	84	125799	45.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.22%
26) 1,2-Dichloroethane-d4	5.09	65	87559	46.96	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.92%
32) Benzene-d6	5.11	84	260939	50.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.50%
36) 1,2-Dichloropropane-d6	6.12	67	88987	49.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.74%
41) Toluene-d8	7.36	98	238591	50.61	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.22%
43) trans-1,3-Dichloropropene-	7.67	79	41901	47.85	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.70%
47) 2-Hexanone-d5	8.14	63	80655	85.70	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.70%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	110456	45.25	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.50%
64) 1,2-Dichlorobenzene-d4	11.68	152	74002	50.05	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.10%


Target Compounds					Ovalue
13) Acetone	2.19	43	12245	12.839 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102518\
Data File : VV008415.D
Acq On : 25 Oct 2018 17:54
Operator : SY/MD
Sample : J5635-20
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A40C0

Quant Time: Oct 26 00:13:39 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 25 23:17:12 2018
Response via : Initial Calibration

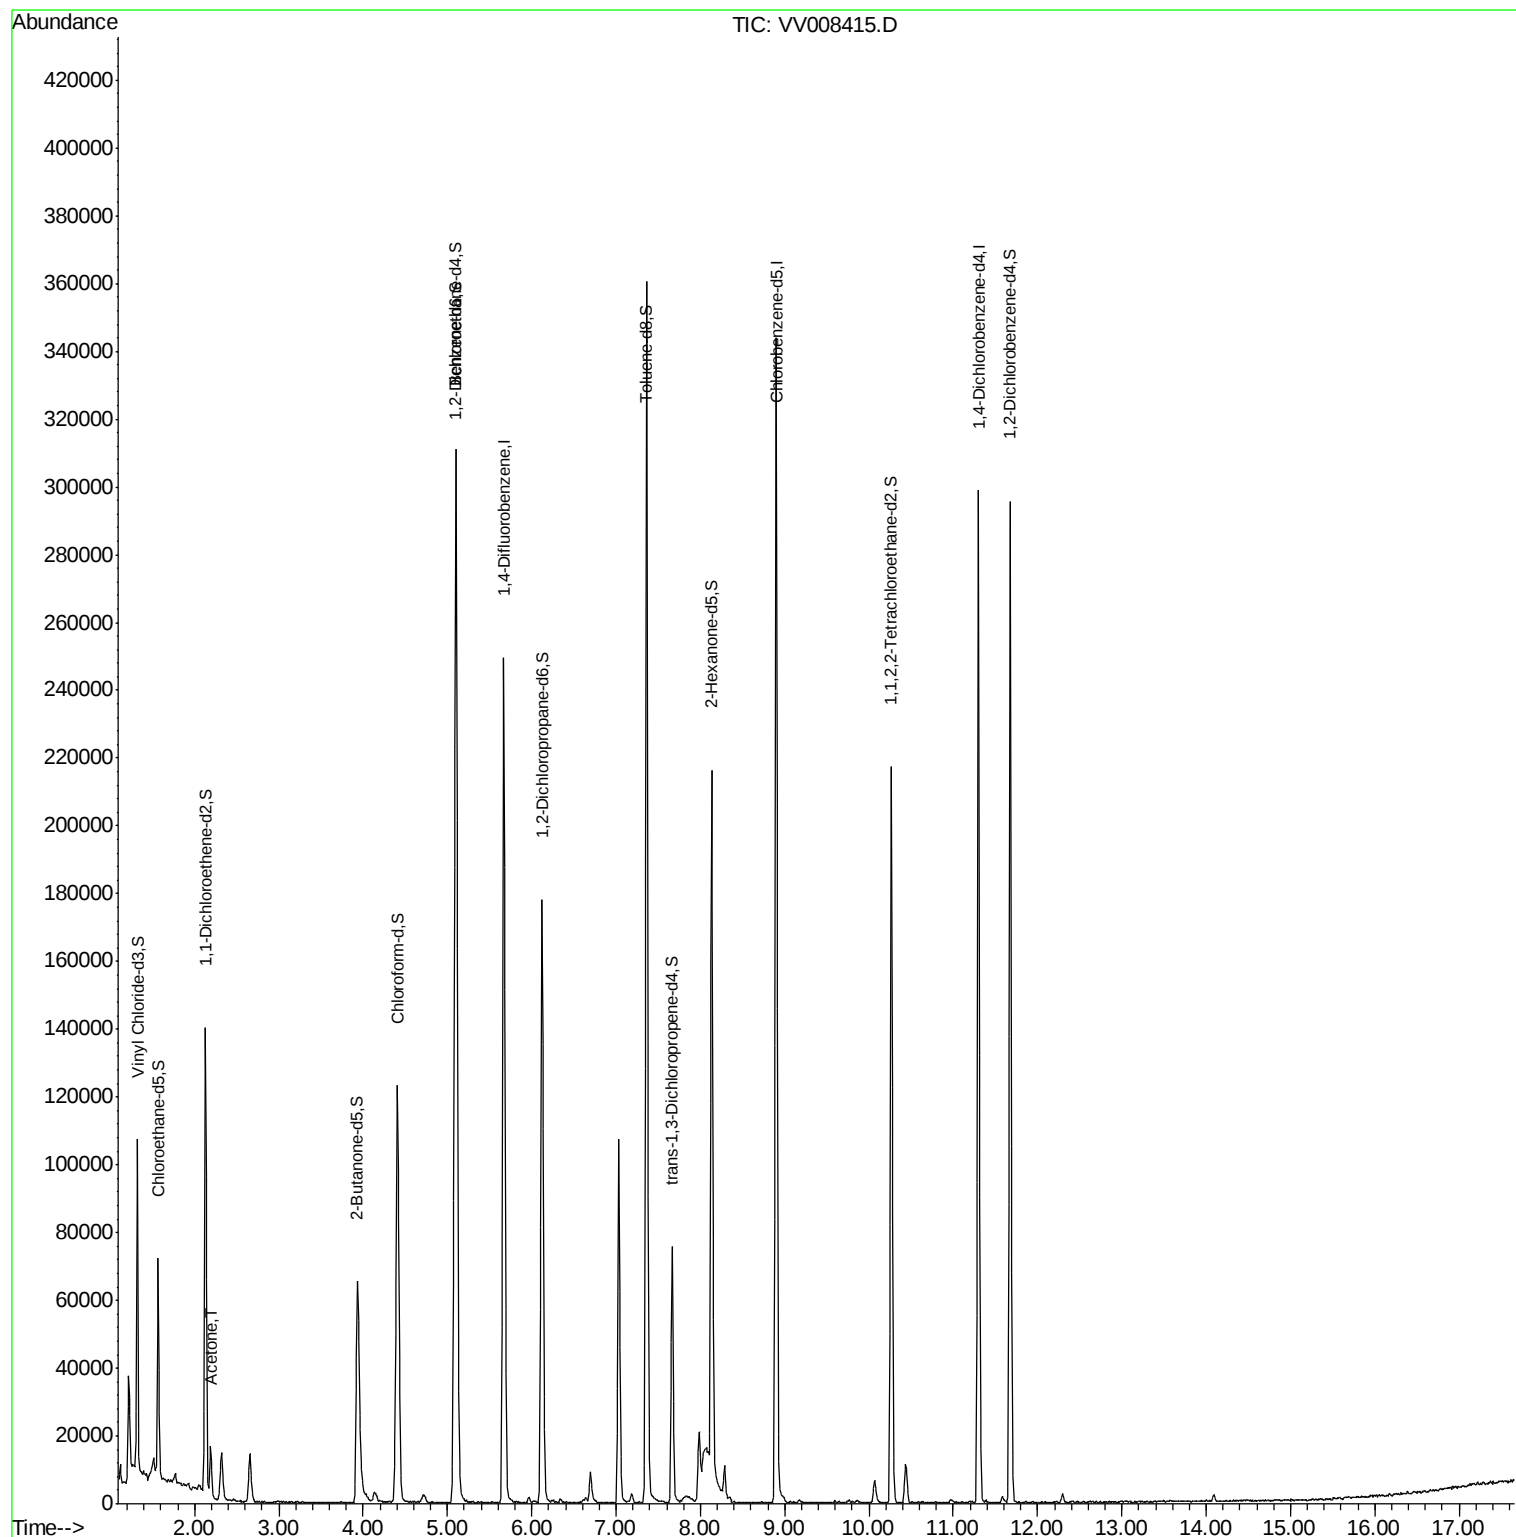

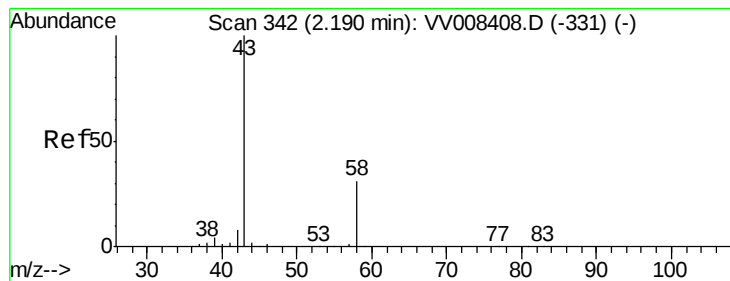

#13

Acetone

Concen: 12.839 ug/L

RT: 2.19 min Scan# 342

Delta R.T. -0.00 min

Lab File: VV008415.D

Acq: 25 Oct 2018 17:54

Instrument :
MSVOA_V
ClientSampleId :
A40C0

Tot Ion: 43 Resp: 12245

Ion Ratio Lower Upper

43 100

58 30.4 0.0 61.4

