

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102518\
 Data File : VV008418.D
 Acq On : 25 Oct 2018 19:04
 Operator : SY/MD
 Sample : J5669-09
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBY7

Quant Time: Oct 26 00:23:34 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 25 23:17:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	199393	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	179305	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	73095	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	54758	49.60	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	99.20%
7) Chloroethane-d5	1.57	69	39364	49.38	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.76%
11) 1,1-Dichloroethene-d2	2.13	63	71323	35.77	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.54%
21) 2-Butanone-d5	3.94	46	107382	89.50	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.50%
24) Chloroform-d	4.41	84	120689	44.32	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.64%
26) 1,2-Dichloroethane-d4	5.09	65	84452	46.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.78%
32) Benzene-d6	5.10	84	251103	49.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.28%
36) 1,2-Dichloropropane-d6	6.12	67	84616	47.71	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.42%
41) Toluene-d8	7.36	98	227314	49.00	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.00%
43) trans-1,3-Dichloropropene-	7.67	79	39902	46.31	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.62%
47) 2-Hexanone-d5	8.14	63	80890	87.34	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.34%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	108727	45.26	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.52%
64) 1,2-Dichlorobenzene-d4	11.68	152	73074	48.87	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.74%


Target Compounds					Ovalue
13) Acetone	2.19	43	5262	5.651 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102518\
Data File : VV008418.D
Acq On : 25 Oct 2018 19:04
Operator : SY/MD
Sample : J5669-09
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBY7

Quant Time: Oct 26 00:23:34 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 25 23:17:12 2018
Response via : Initial Calibration

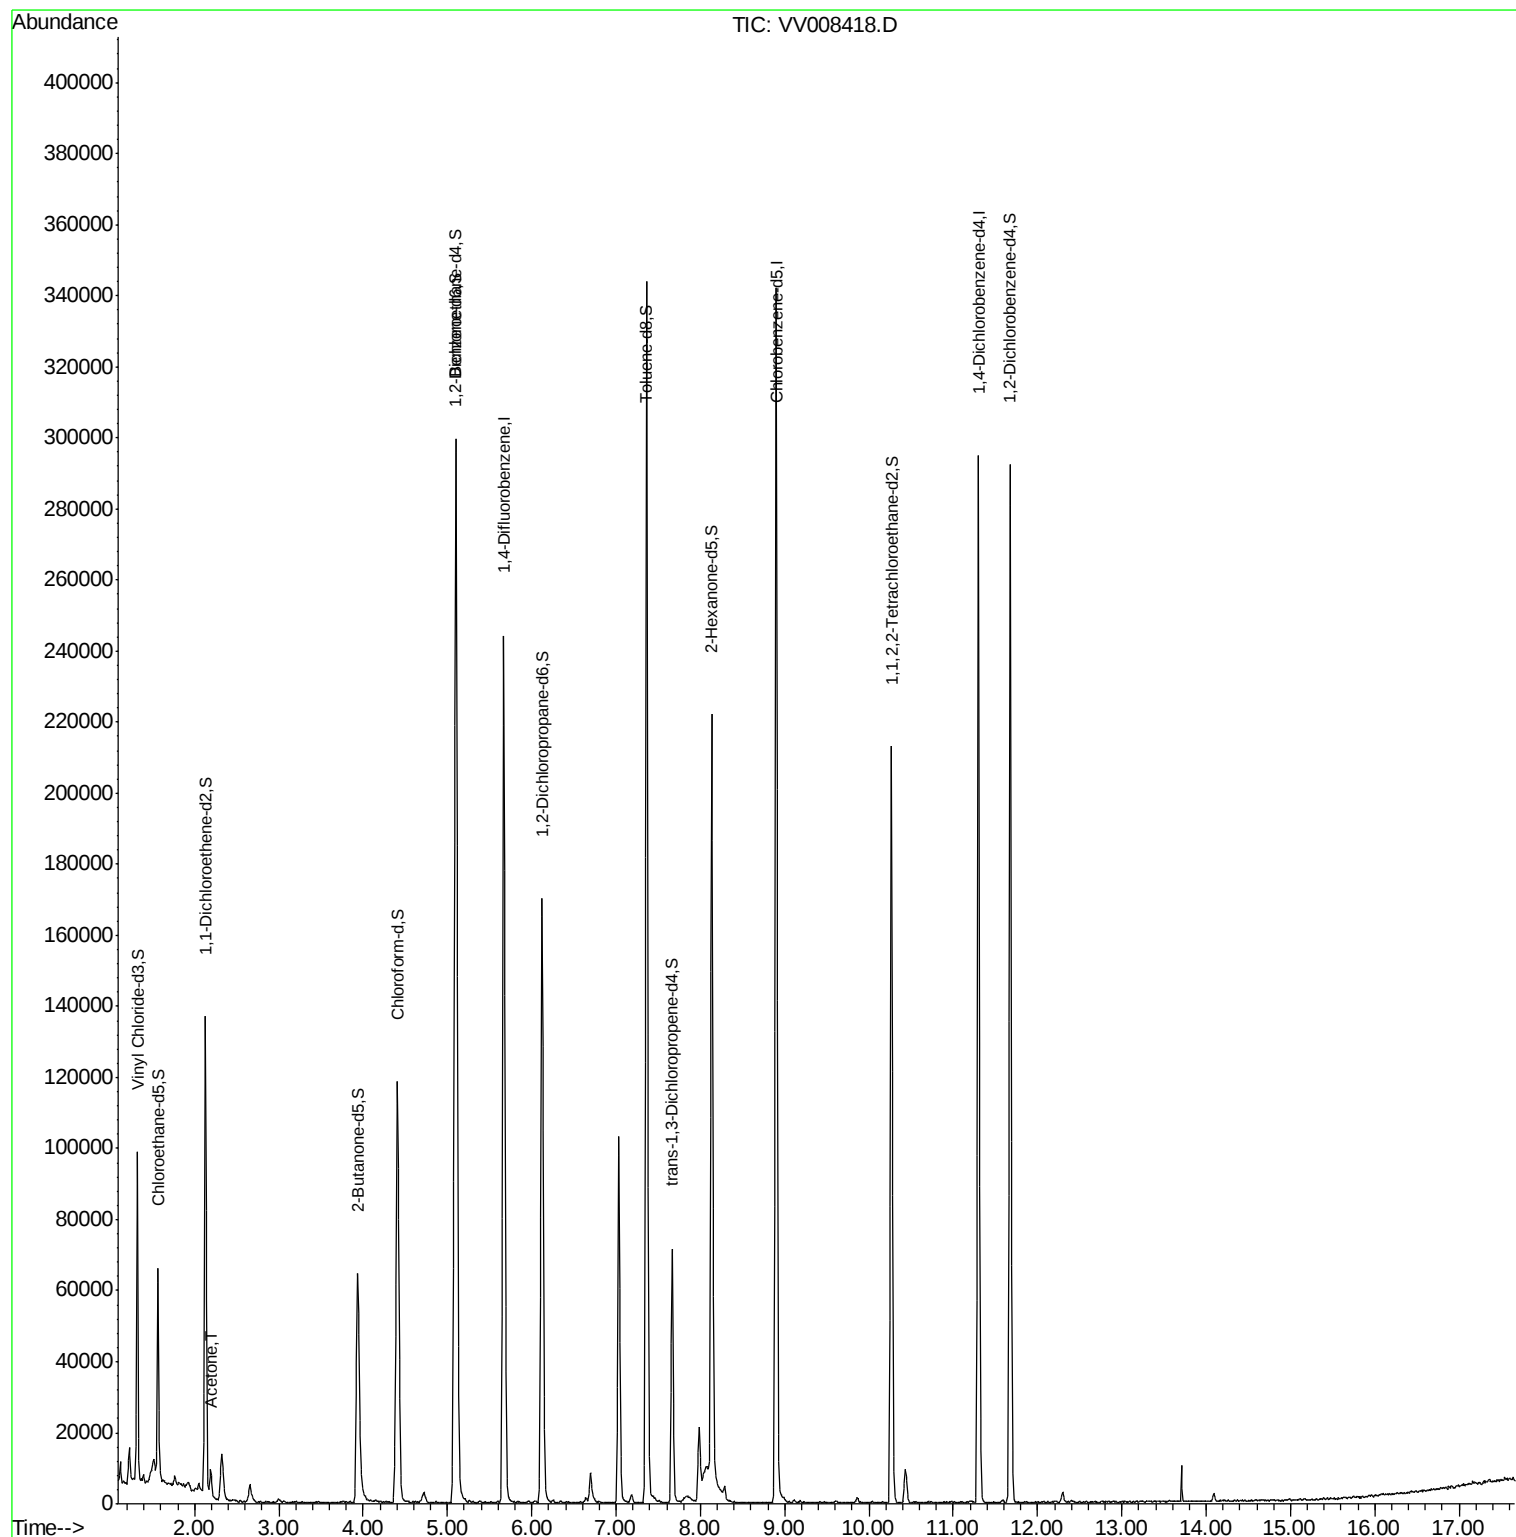

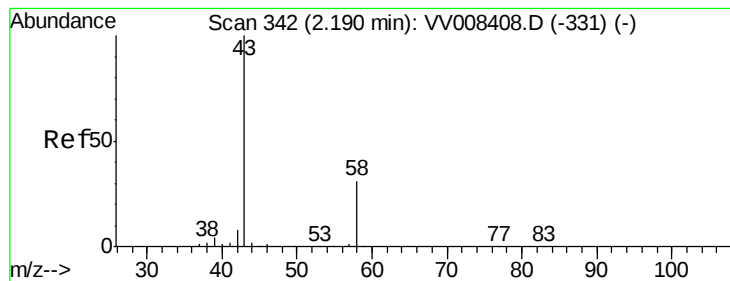

#13

Acetone

Concen: 5.651 ug/L

RT: 2.19 min Scan# 343

Delta R.T. 0.00 min

Lab File: VV008418.D

Acq: 25 Oct 2018 19:04

Instrument :
MSVOA_V
ClientSampleId :
ETBY7

Tot Ion: 43 Resp: 5262

Ion Ratio Lower Upper

43 100

58 32.3 0.0 61.4

