

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102519\
Quantitation Report (QT Reviewed)

Data File : VV013335.D


Acq On : 25 Oct 2019 00:06
Operator : SY/MD
Sample : K5462-20
Misc : 25.0ML/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0G24

Manual Integrations
APPROVED

MMDadoda
10/26/2019 10:04:20 AM

Quant Time: Oct 25 05:54:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 25 04:42:43 2019
Response via : Initial Calibration

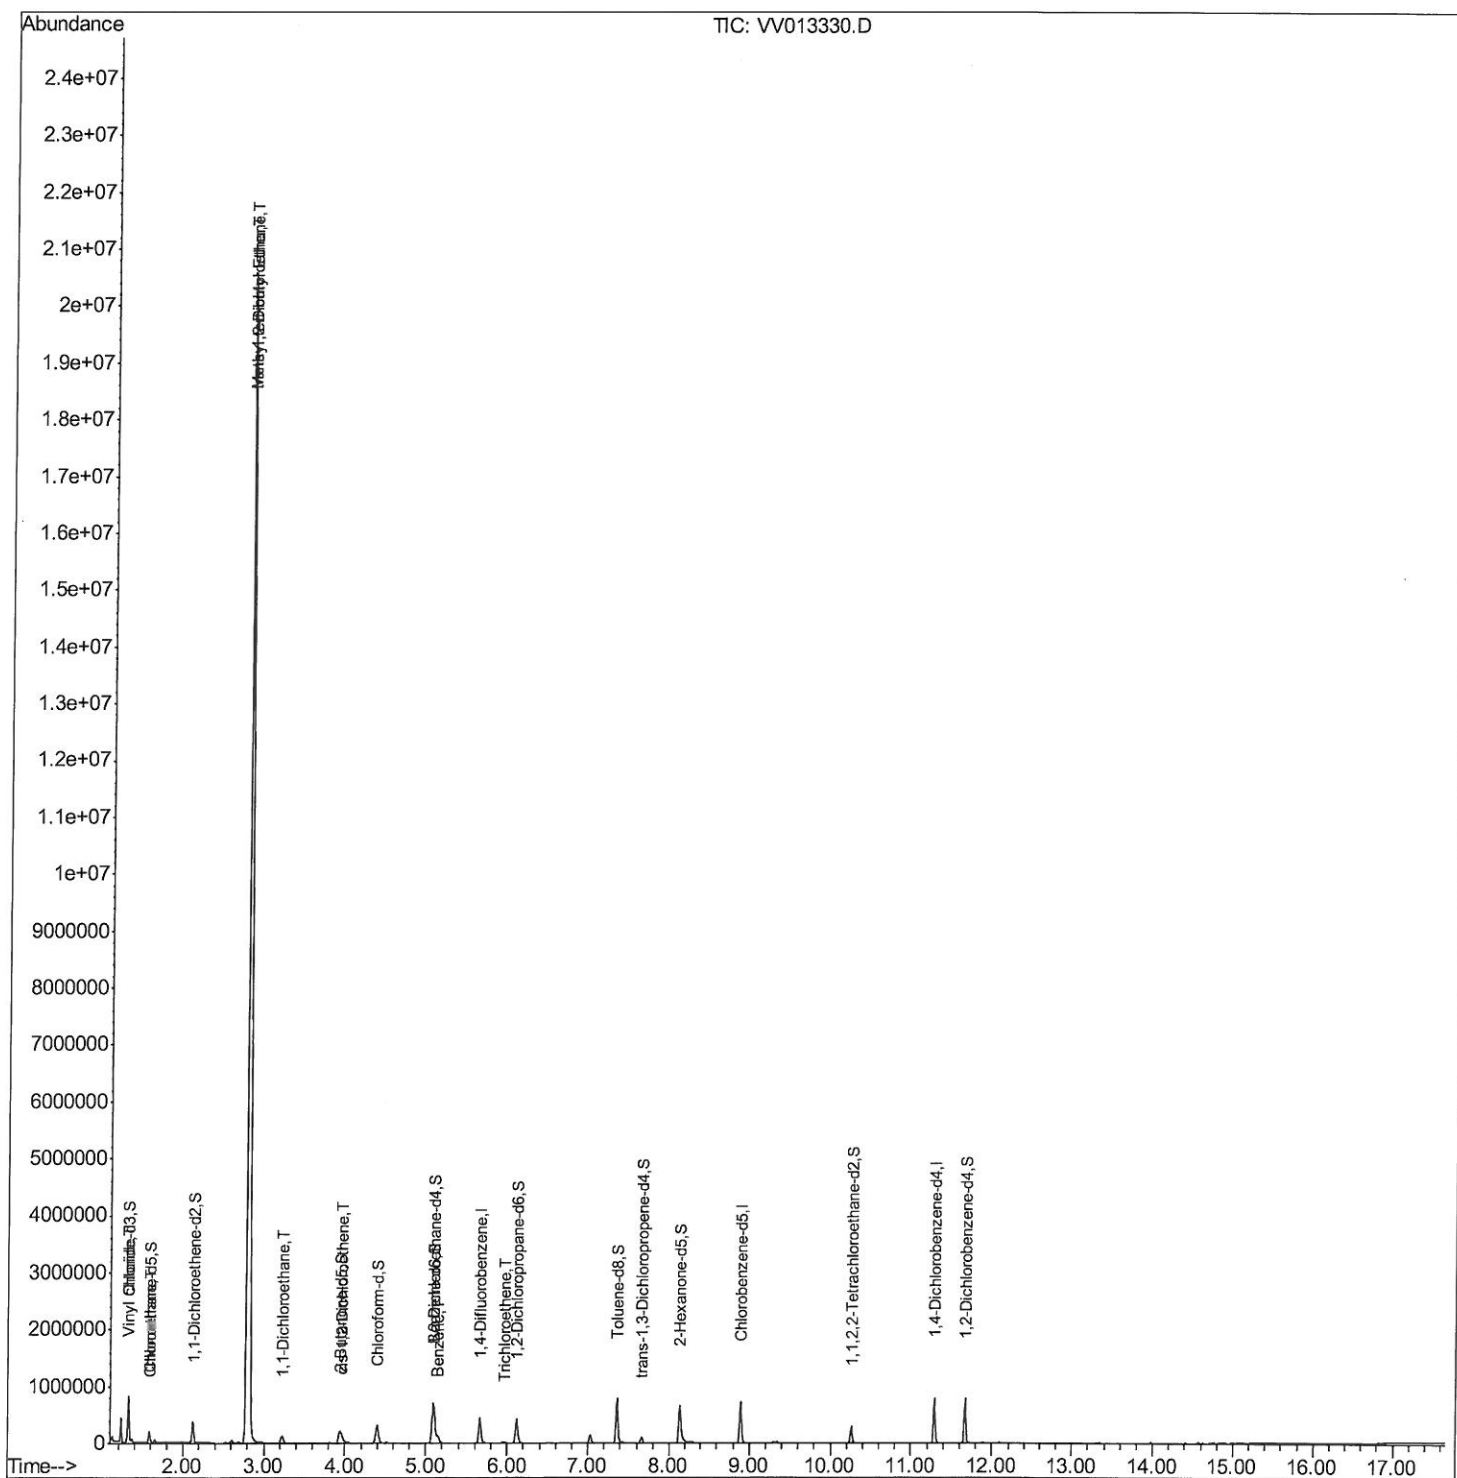

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102519\
Quantitation Report (Qedit)

Data File : VV013335.D




Acq On : 25 Oct 2019 00:06
Operator : SY/MD
Sample : K5462-20
Misc : 25.0ML/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0G24

Manual Integrations
APPROVED

MMDadoda
10/26/2019 10:04:20 AM

Quant Time: Oct 25 04:47:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 25 04:42:43 2019
Response via : Initial Calibration

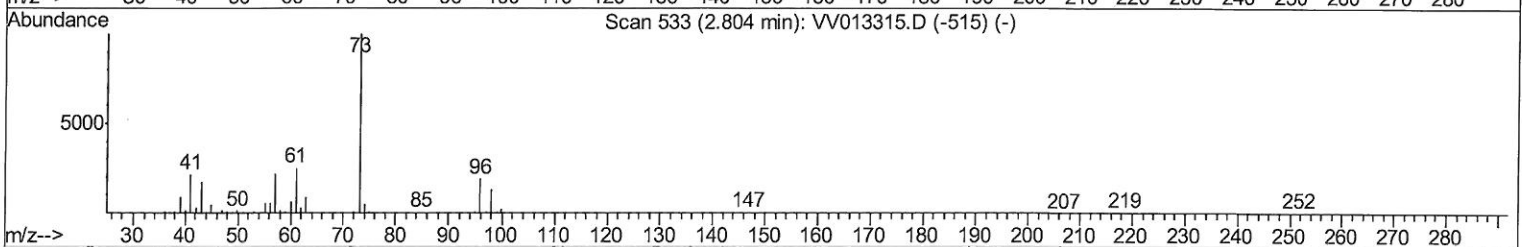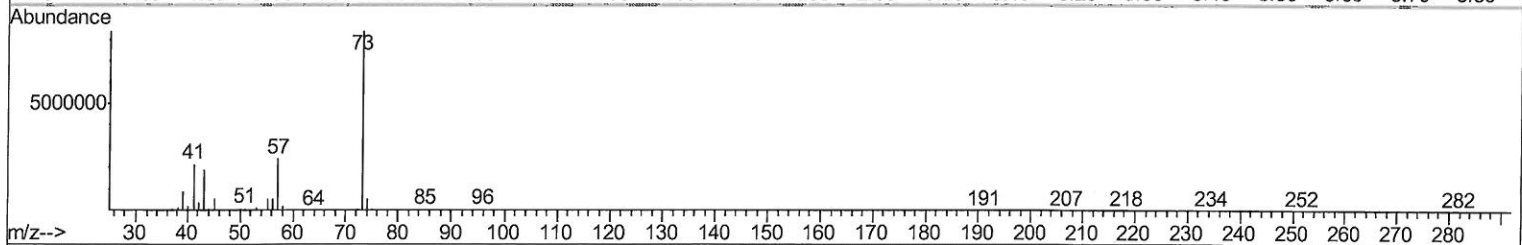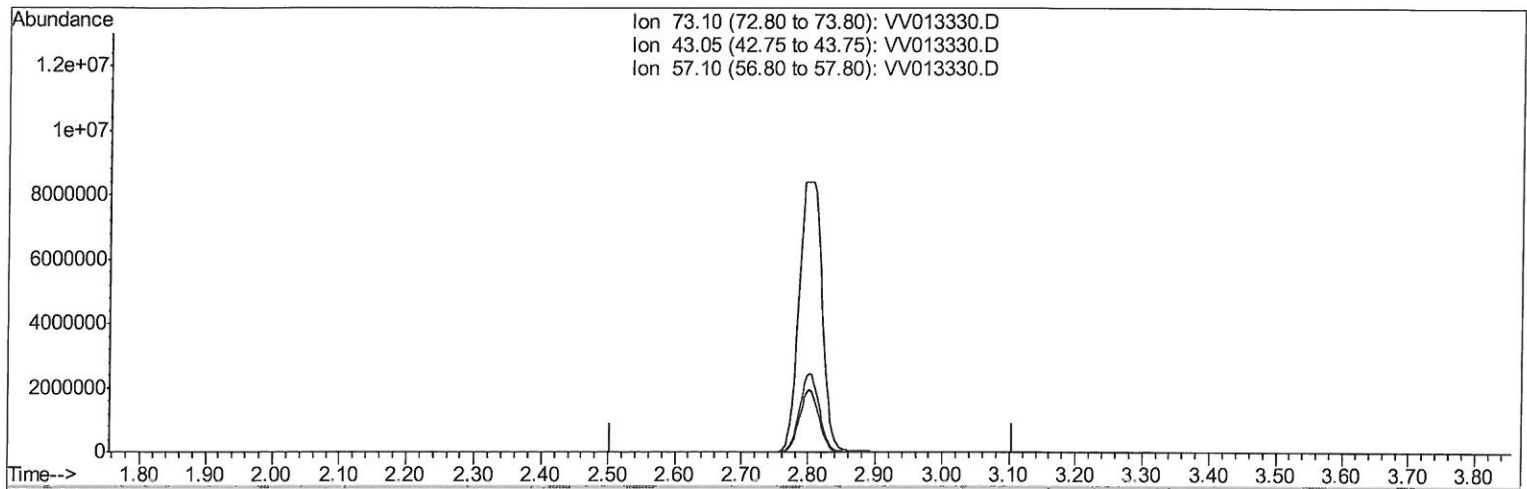

TIC: VV013330.D

(17) Methyl tert-butyl Ether (T)

2.804min (-2.804) 0.00ug/L

response 0

Ion	Exp%	Act%
73.10	100	0.00
43.05	16.40	0.00#
57.10	20.50	0.00#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102519\
Quantitation Report (Qedit)

Data File : VV013335.D




Acq On : 25 Oct 2019 00:06
Operator : SY/MD
Sample : K5462-20
Misc : 25.0ML/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0G24

Manual Integrations
APPROVED

MMDadoda
10/26/2019 10:04:20 AM

Quant Time: Oct 25 04:47:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 25 04:42:43 2019
Response via : Initial Calibration

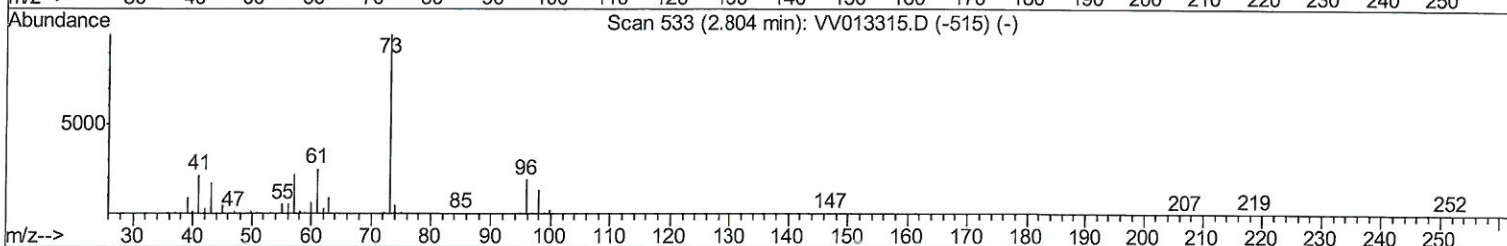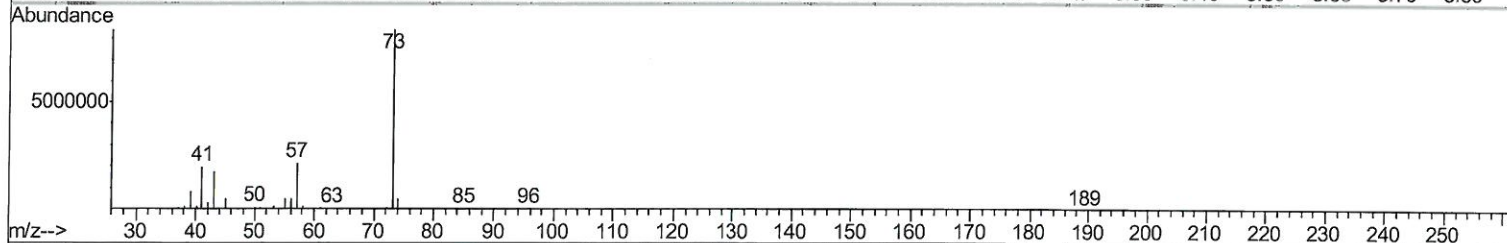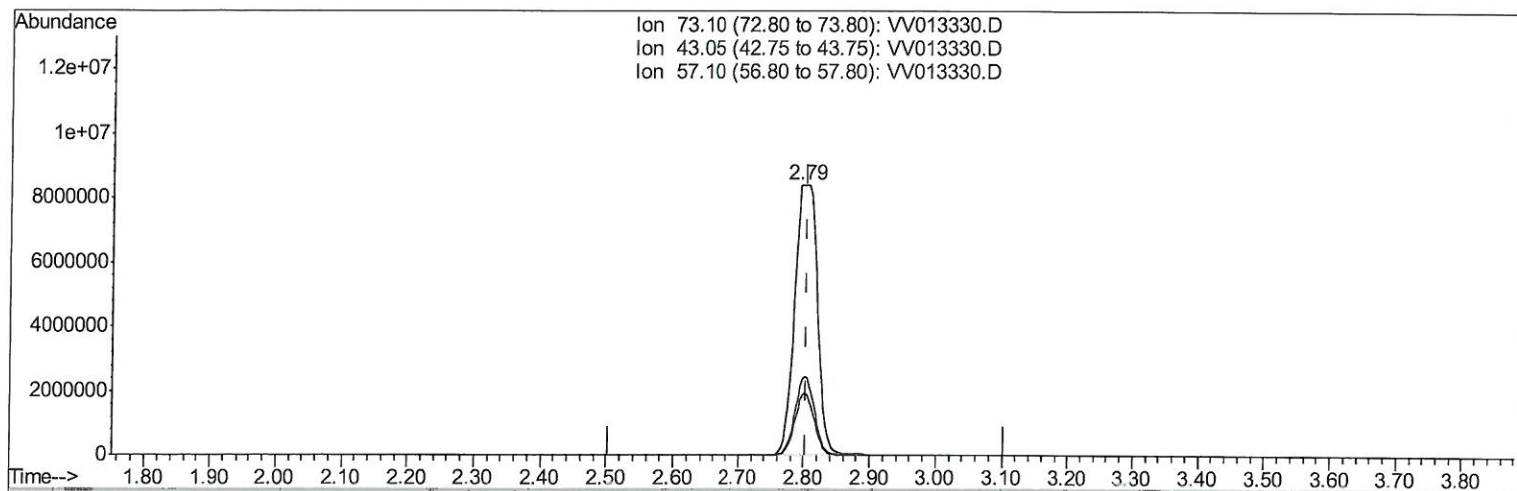

TIC: VV013330.D

(17) Methyl tert-butyl Ether (T)

2.794min (-0.010) 279.18ug/L m

response 20135514

Ion	Exp%	Act%
73.10	100	100
43.05	16.40	0.00#
57.10	20.50	0.00#
0.00	0.00	0.00

7 mQ
10/26/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102519\
Quantitation Report (QT Reviewed)

Data File : VV013335.D

Acq On : 25 Oct 2019 00:06
Operator : SY/MD
Sample : K5462-20
Misc : 25.0ML/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0G24

Manual Integrations
APPROVED

MMDadoda
10/26/2019 10:04:20 AM

Quant Time: Oct 25 05:54:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 25 04:42:43 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.66	114	396099	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	430200	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	226039	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	152057	5.21	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.20%
7) Chloroethane-d5	1.58	69	127387	5.29	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.80%
11) 1,1-Dichloroethene-d2	2.13	63	186352	3.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.80%
20) 2-Butanone-d5	3.93	46	326227	58.17	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.34%
24) Chloroform-d	4.40	84	323404	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
26) 1,2-Dichloroethane-d4	5.08	65	155193	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.60%
32) Benzene-d6	5.10	84	658130	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
36) 1,2-Dichloropropane-d6	6.12	67	200607	4.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.80%
41) Toluene-d8	7.36	98	522757	4.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.00%
43) trans-1,3-Dichloropropene-	7.66	79	56615	3.57	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.40%
46) 2-Hexanone-d5	8.13	63	205171	36.30	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	72.60%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	140899	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	228810	5.20	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.00%

Target Compounds

						Qvalue
5) Vinyl chloride	1.32	62	163010	4.264	ug/L	99
8) Chloroethane	1.60	64	4689	0.206	ug/L	91
17) Methyl tert-butyl Ether	2.79	73	20135514m	279.178	ug/L	
18) trans-1,2-Dichloroethene	2.79	96	52057	1.418	ug/L	92
19) 1,1-Dichloroethane	3.23	63	127442	2.136	ug/L	98
22) cis-1,2-Dichloroethene	3.96	96	30101	0.766	ug/L #	91
33) Benzene	5.15	78	128062	0.780	ug/L	100
34) Trichloroethene	5.96	95	5281	0.120	ug/L	84

7 MD
10/26/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed